


**Data file:** E:\DATA\181229\20181229 2018-12-29 11-45-16\Compstatin-01.D  
**Sample name:** Compstatin-01  
**Description:** Mobile phase: Buffer A: 0.1%TFA in H2O  
 Buffer B: 0.1%TFA in ACN  
 Gradient: 18-28% unitary C18, 4.6\*150mm, 5um 100A (A-005)  
 Instrument: Agilent HPLC 1100

**Instrument:** QC **Location:** 92  
**Injection date:** 2018/12/29 13:19:06 **Injection:** 1 of 1  
**Last changed:** 2018/12/29 13:05:38 **Injection volume:** 5.000  
**Acq. operator:** QC\_1

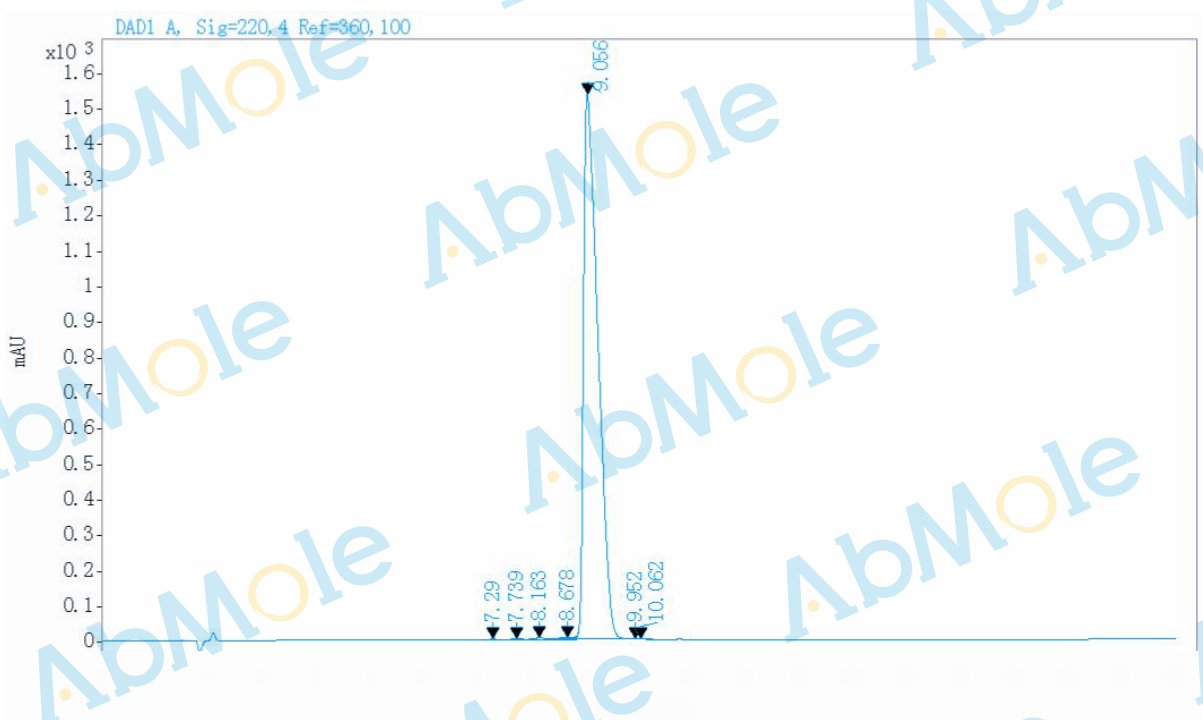

**Signal:** DAD1 A, Sig=220,4 Ref=360,100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
7.290	BB	0.1867	20.9953	1.6701	0.0733	
7.739	BB	0.1464	28.3162	3.1053	0.0989	
8.163	BV E	0.2413	56.7314	3.8184	0.1982	
8.678	VV E	0.2864	119.3689	6.1512	0.4170	
9.056	VB R	0.2922	28375.6484	1530.9578	99.1269	
9.952	BV F	0.1275	8.5510	1.0445	0.0299	
10.062	VB	0.1553	15.9527	1.6729	0.0557	
	Sum		28625.5640			