


=====

Acq. Operator	: SYSTEM	Seq. Line	: 4
Acq. Instrument	: HPLC-030	Location	: 9
Injection Date	: 11/10/2019 11:03:42 AM	Inj	: 1
		Inj Volume	: 10.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.000 µl			
Acq. Method	: D:\HPLC-030\Data\2019\20191110 2019-11-10 09-48-02\M-A70B30.M		
Last changed	: 11/10/2019 10:38:07 AM by SYSTEM		
Analysis Method	: D:\HPLC-030\METHODS\SUNFIRE C18 5UM 4.6X150MM\M-AB.M		
Last changed	: 11/10/2019 11:37:06 AM by SYSTEM		
Method Info	: SunFire C18 5um 4.6x150mm 25C 1.000ml/min 16min		
	Mobile Phase A: 0.03%TFA in H2O, Mobile Phase B: 0.03%TFA in ACN.		

=====

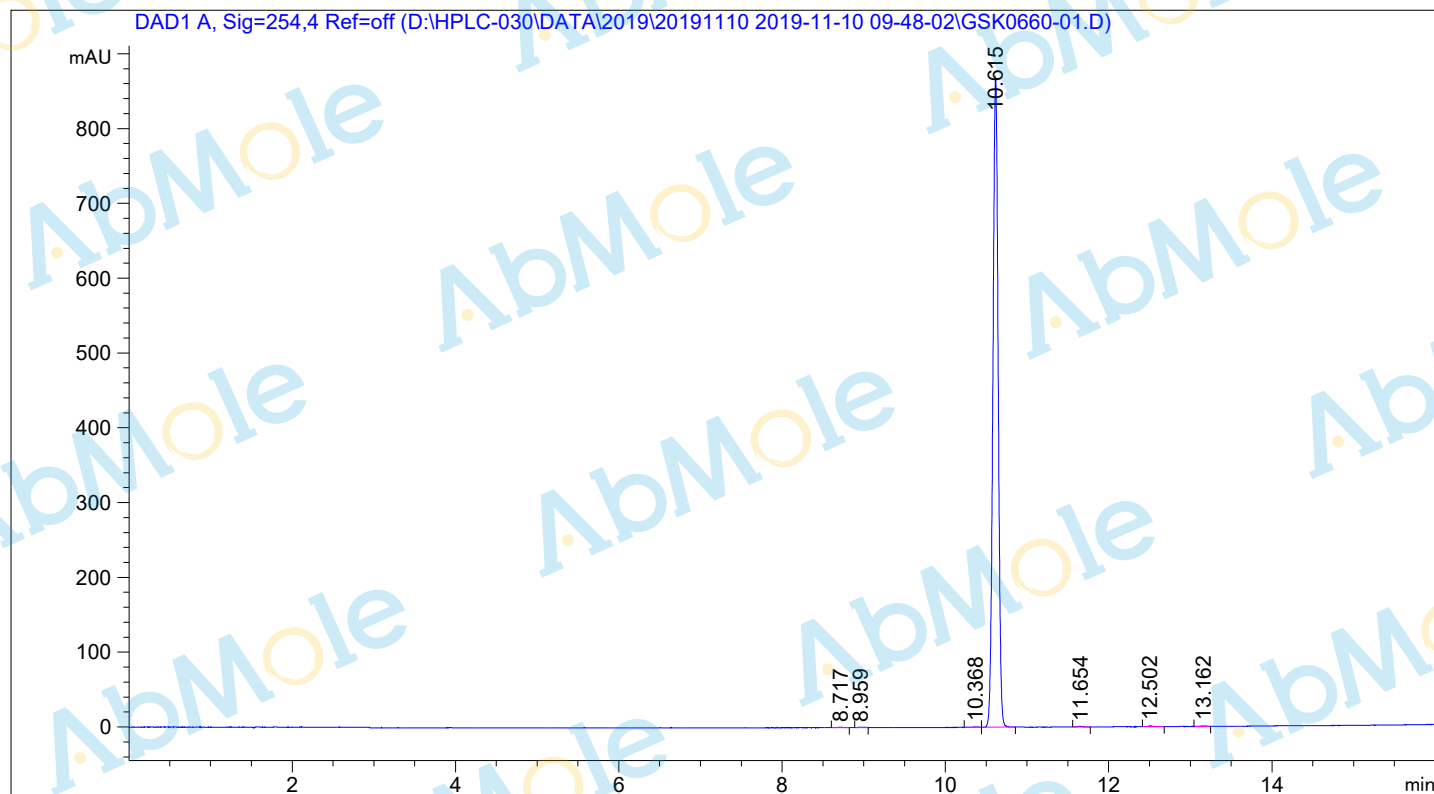

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.717	BB	0.0621	2.91867	6.07184e-1	0.0746
2	8.959	BB	0.0631	1.69053	3.28377e-1	0.0432
3	10.368	BB	0.0646	2.60652	5.09976e-1	0.0666
4	10.615	BB	0.0694	3893.40088	867.36420	99.4661
5	11.654	BB	0.0657	4.47834	8.46823e-1	0.1144
6	12.502	BB	0.0732	5.25950	8.74411e-1	0.1344
7	13.162	BB	0.0629	3.94399	8.22908e-1	0.1008

Totals : 3914.29844 871.35388

=====
*** End of Report ***