

File D:\DATA

Injection Date : 28 Jul 14 06:45 pm

Sample Name : GSK2636771

Acq. Operator : XXXX

Spec. Reported : MS Integration

Acq. Method : D:\METHODS\1-POS-3MIN.M

Analysis Method : D:\METHODS\1-POS-3MIN.M

Sample Info : Easy-Access Method: '1-POS-3MIN'

Method Info : Mobile Phase: A: water (0.01%TFA) B:ACN(0.01%TFA)

Gradient: 5% to 95%B within 1.4 min

Flow Rate :2.0ml/min

Column :SunFire C18, 4.6\*50mm,3.5um


Oven Temperature : 50C

Location :


Inj : 1

Inj Volume : 1 ul


\*ADC1 A, ADC1 CHANNEL A

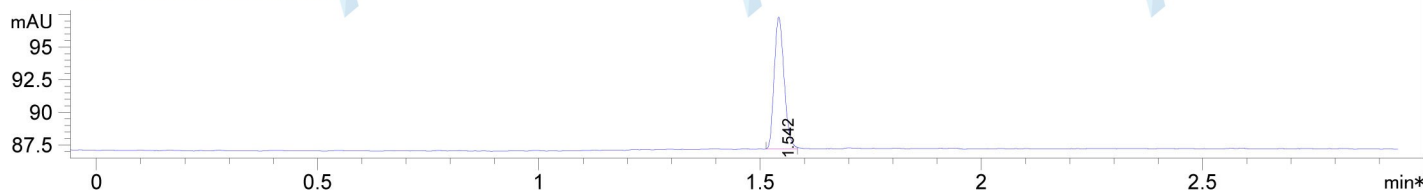


DAD1 A, Sig=214,4 Ref=off

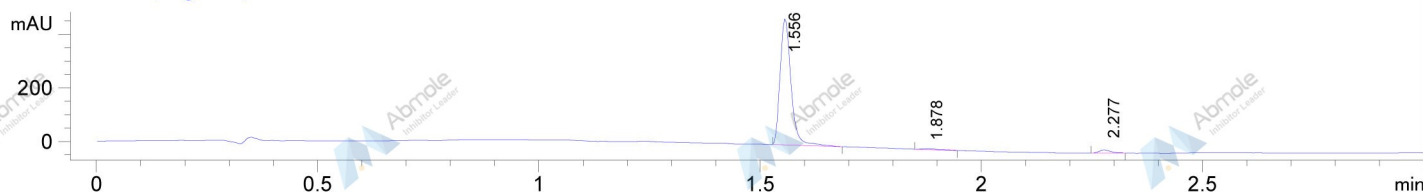

DAD1 B, Sig=254,4 Ref=off

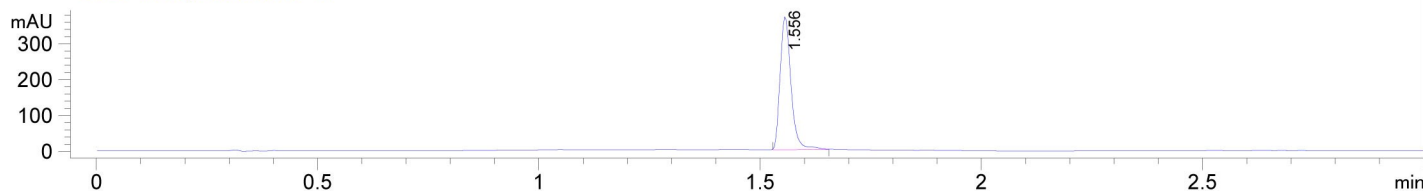

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

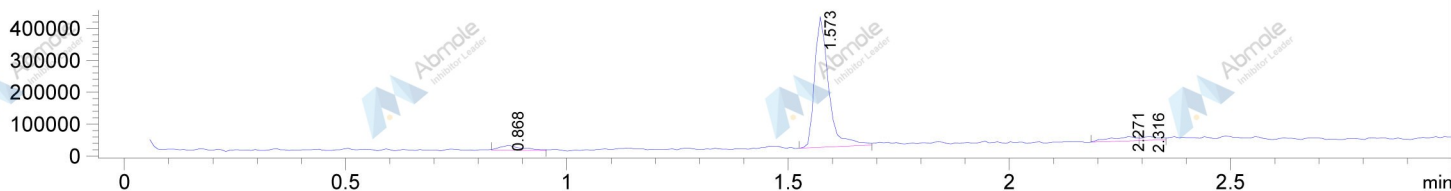

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.56	0.03	810.80	473.19	96.00
1.88	0.03	9.73	3.98	1.15
2.28	0.03	24.07	12.63	2.85

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
1.56	0.03	634.02	372.12	100.00

Ret. Time: 0.87


<<<< POSITIVE SPECTRA >>>>

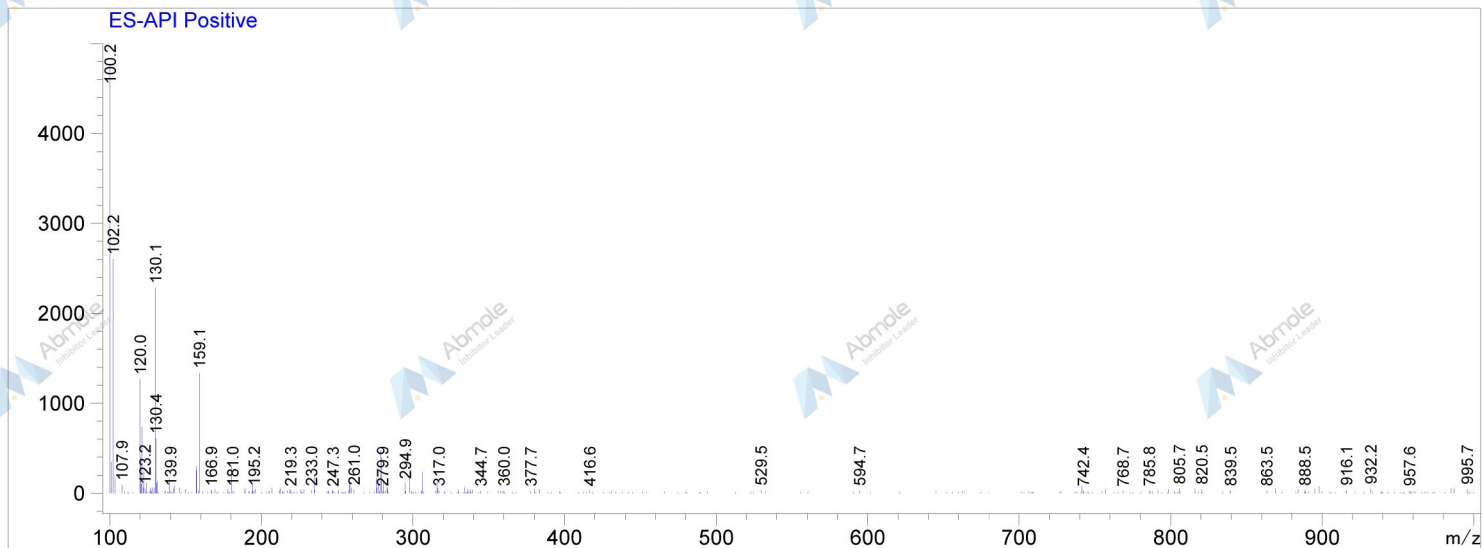

Ret. Time: 1.57

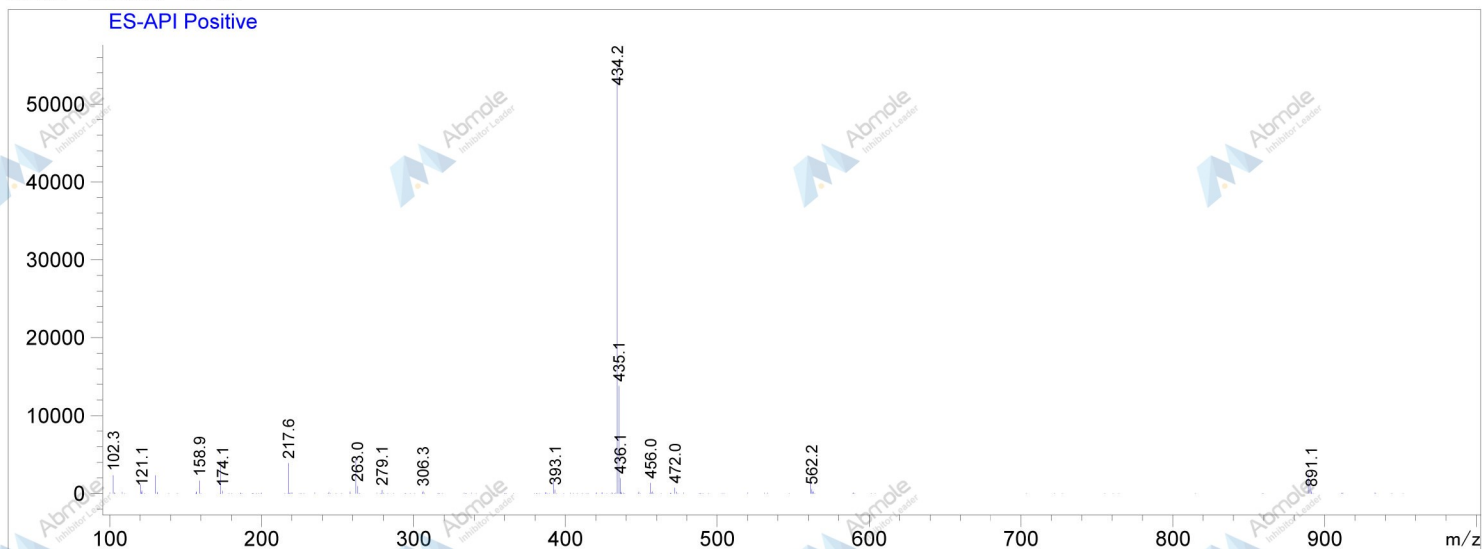

Ret. Time: 2.27

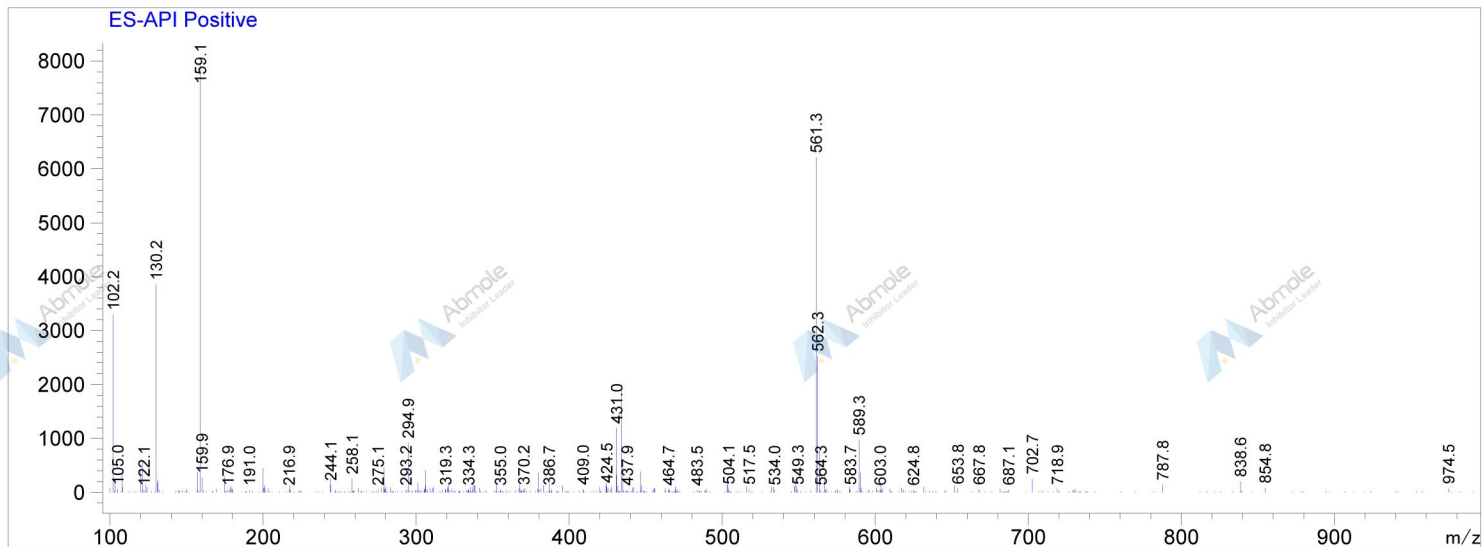

Ret. Time: 2.32

ES-API Positive

