

Openlynx Report UPLCMS-21-REPORT

Vial:1:37

Injection Volume:0.1000

Time:10:40:48

Sample: M10081-Omaveloxolone-02

MS Method:2-5min-100-1000

UserName:

File:474034-05-3

Date:22-Oct-2021

Instrument:ACQ-SQD2#LCA316

Inlet Method:2-5min-05-95

Method:0709test.olp

Printed: Fri Oct 22 10:43:58 2021


Sample Report:

Sample:M10081-Omaveloxolone-02


Vial 1:37 ID 474034-05-3

Date 22-Oct-2021 Time 10:40:48

2: UV Detector: 214

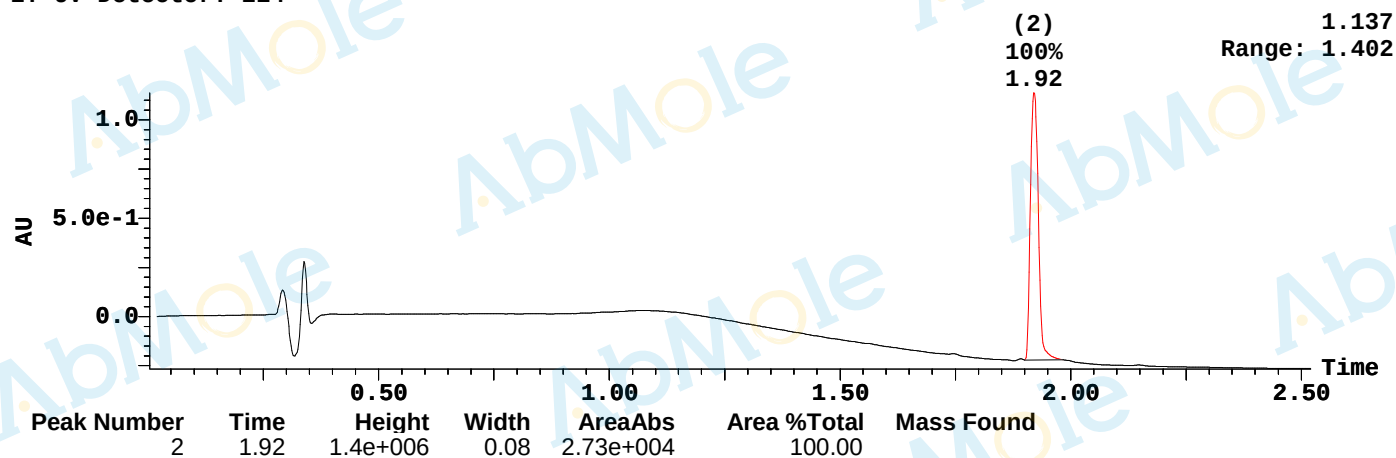

2: UV Detector: 254

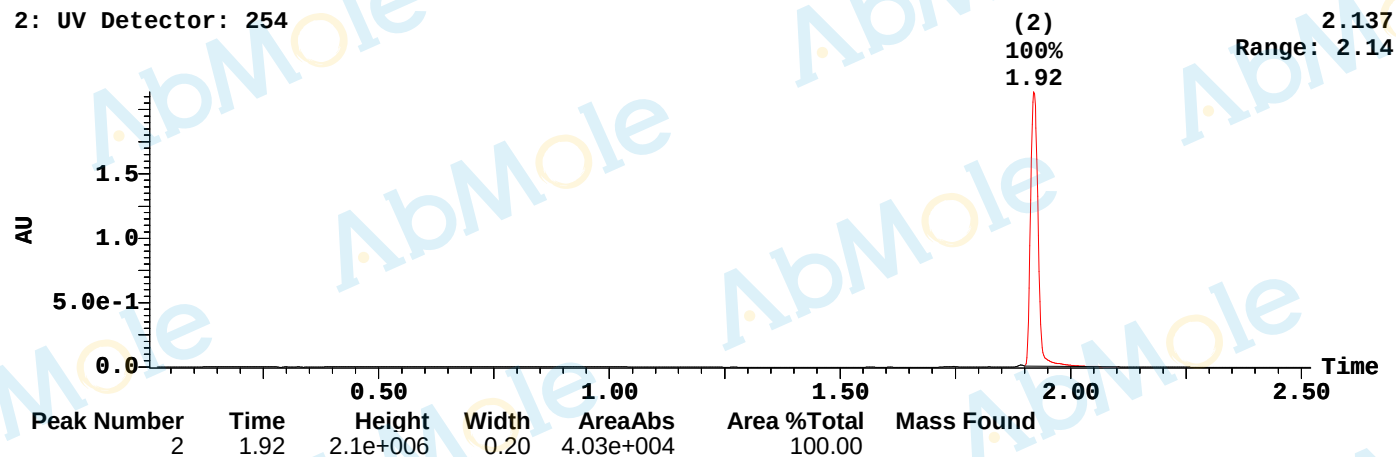

Openlynx Report UPLCMS-21-REPORT


Vial:1:37
Injection Volume:0.1000
Time:10:40:48
Sample: 50
MS Method:2-5min-100-1000
UserName:

File:474034-05-3
Date:22-Oct-2021
Instrument:ACQ-SQD2#LCA316
Inlet Method:2-5min-05-95
Method:0709test.olp

Printed: Fri Oct 22 10:43:58 2021

Sample Report (continued):


1: MS ES+ :TIC Smooth (Mn, 7x3)

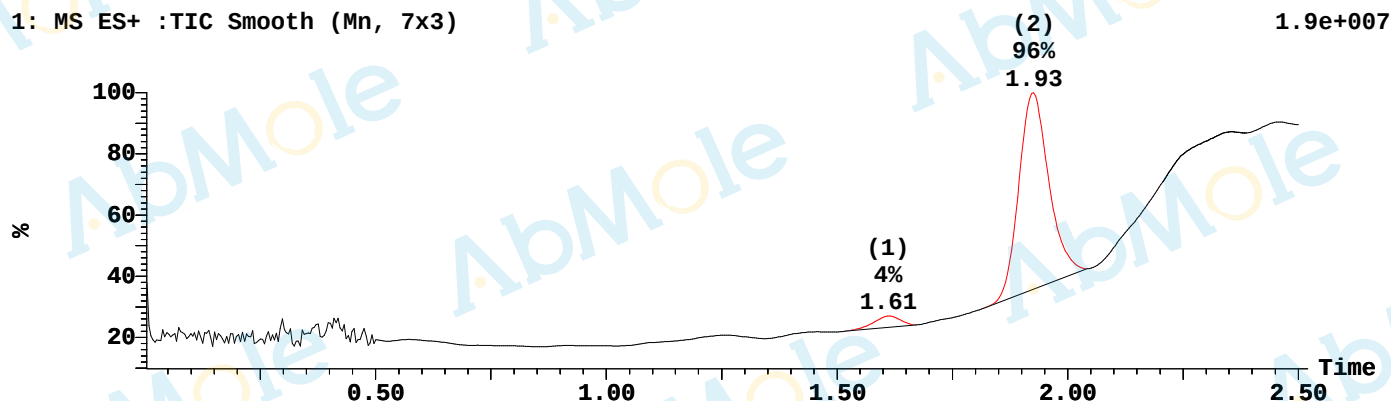

Time
1.61

1: (Time: 1.61) Combine (361:385-(327:337+409:419))

1: MS ES+
4.0e+005

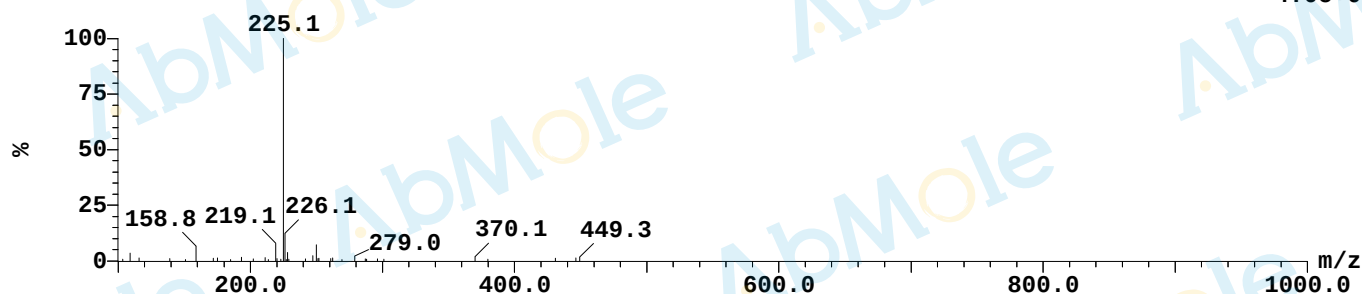

Time
1.93

2: (Time: 1.93) Combine (434:458-(400:410+482:492))

1: MS ES+
4.4e+006

