


HPLC REPORT

Data file: D:\CHEM32\1\DATA\220520\22040081-1Final.D
Sample name: M10246-Bulevir tide-02
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
Buffer B: 0.1%TFA in ACN
Gradient: 43-53% B in 20min, Flow rate: 1.0ml/min
Column: Unitary C18, 4.6*150mm, 5um 100A
Instrument: Agilent HPLC 1100

Instrument: 1100
Injection date: 2022/5/20 12:57:10
Last changed: 2022/5/20 16:44:18
Location: 82
Injection: 1 of 1
Injection volume: 10.000
Acq. operator: SYSTEM

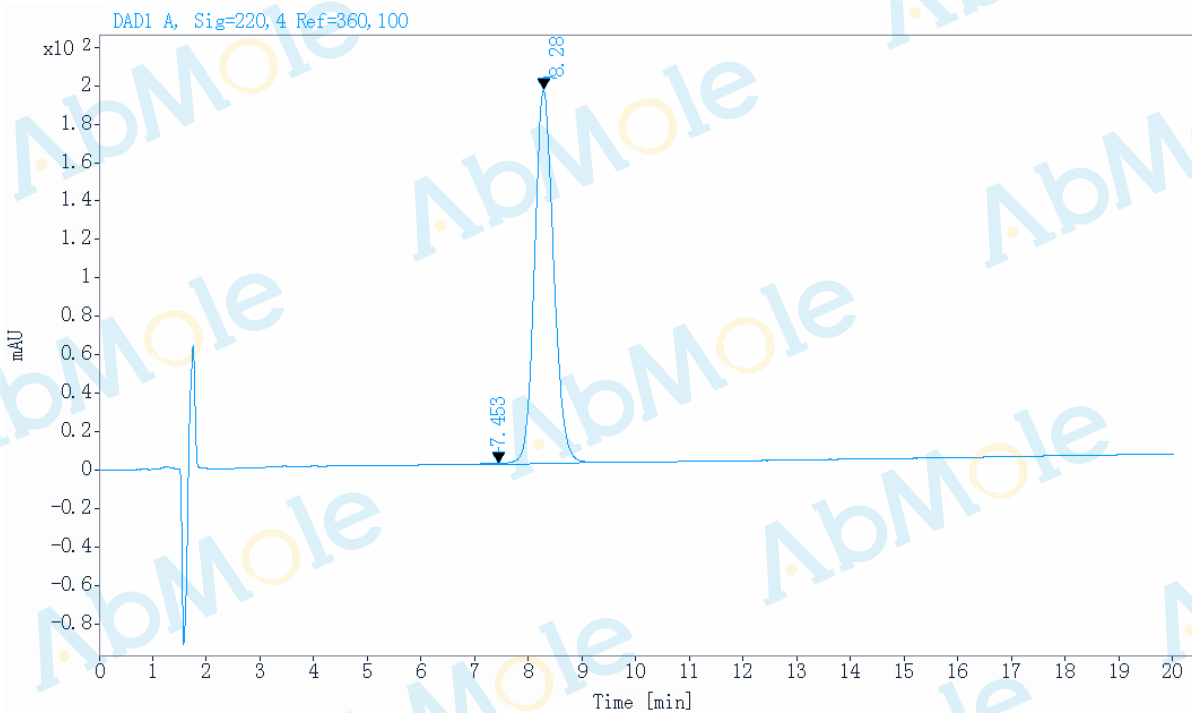

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
7.453	MF	0.4047	14.8516	0.6116	0.3080
8.280	FM	0.4121	4807.4067	194.4341	99.6920
Sum			4822.2584		