


# MASS SPECTROMETRY REPORT

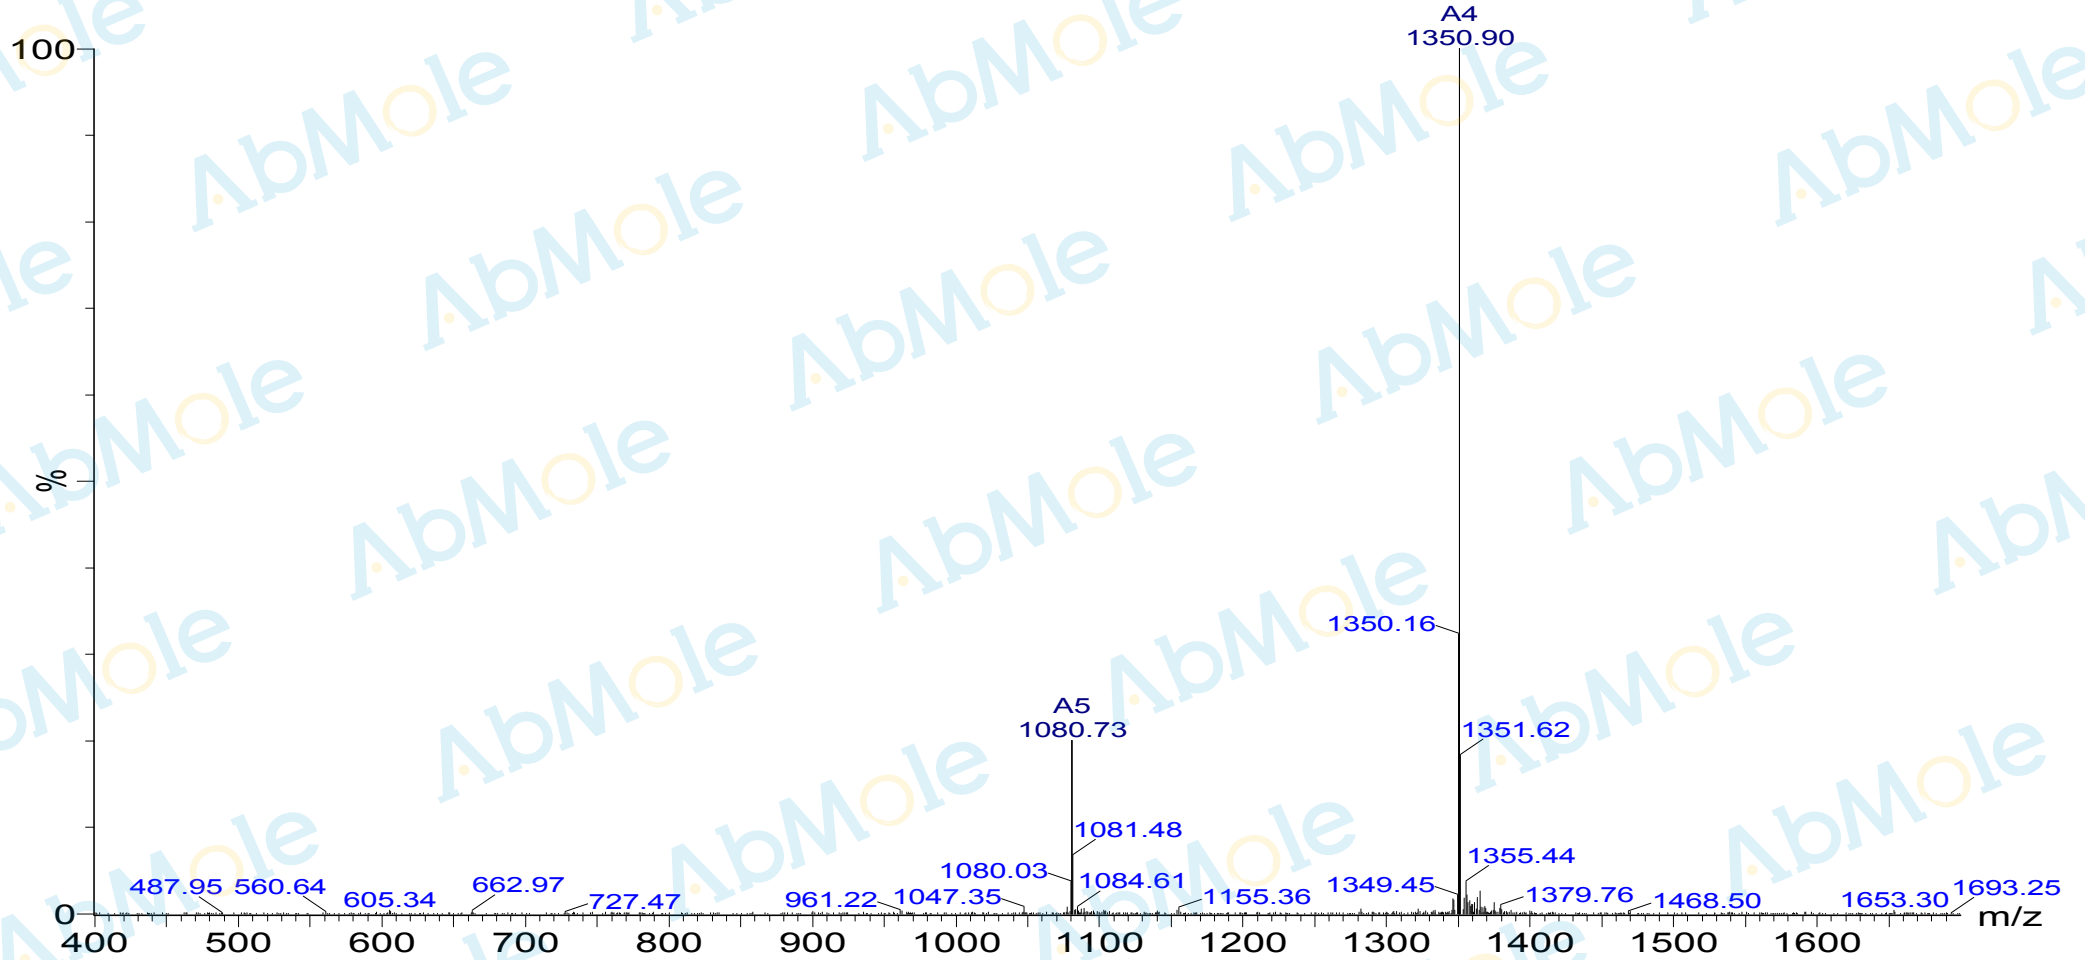

Sample Description

Analyzed date: 2022-05-20

Analyst: SHAO

Sample: M10246-Bulevirtide-02

M.W.: 5398.9

Lot. No.:

Instrument

Probe:

Nebulizer Gas Flow:

CDL:

CDL Temp.:

Block Temp.:

SHIMADZU LCMS-2022

ESI

1.5L/min

-20.0v

250 °C

200 °C

Probe Bias:

Detector:

T. Flow:

B. Conc.:

+4.5kv

1.5kv

0.2ml/min

50%H2O/50%ACN