




Sample name: M10258-SR-4835-01
Instrument: A010
Inj. volume: 5
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

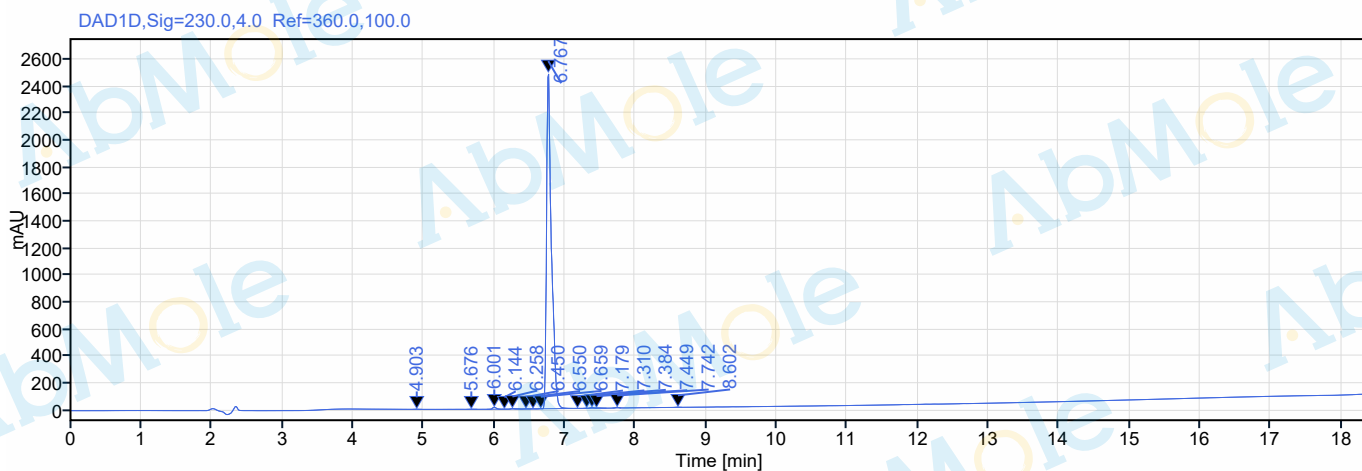

Signal: DAD1D,Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
4.903	BM m	0.13	3.49	1.15	0.03
5.676	BM m	0.15	3.59	0.97	0.03
6.001	BM m	0.21	56.77	14.95	0.47
6.144	MM m	0.09	1.73	0.49	0.01
6.258	BB	0.20	25.62	5.42	0.21
6.450	MM m	0.11	2.66	0.84	0.02
6.550	MM m	0.11	2.58	0.82	0.02
6.659	MM m	0.07	1.93	0.84	0.02
6.767	BB	0.44	11974.93	2486.55	98.74
7.179	MM m	0.09	0.84	0.34	0.01
7.310	MM m	0.07	3.05	1.12	0.03
7.384	MM m	0.11	20.94	4.96	0.17
7.449	MB m	0.15	9.42	2.02	0.08
7.742	MM m	0.12	15.58	4.85	0.13
8.602	MB m	0.12	4.21	1.25	0.03