




Agilent Technologies

Sample name: M10326-Zuranolone-02-1
Instrument: 3
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

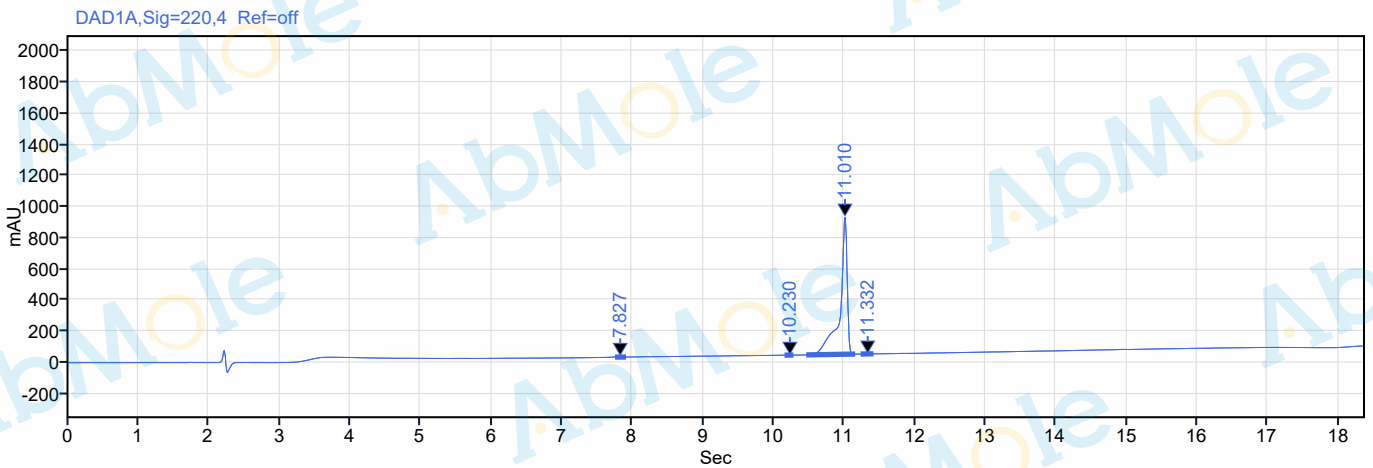

Signal: DAD1A,Sig=220,4 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
7.827		22.4	6.1	0.352
10.230		2.5	0.7	0.040
11.010		6333.6	883.1	99.547
11.332		3.9	0.7	0.061
	Sum	6362.44		