



Agilent Technologies

Sample name: M10326-Zuranolone-03

Instrument: A012

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

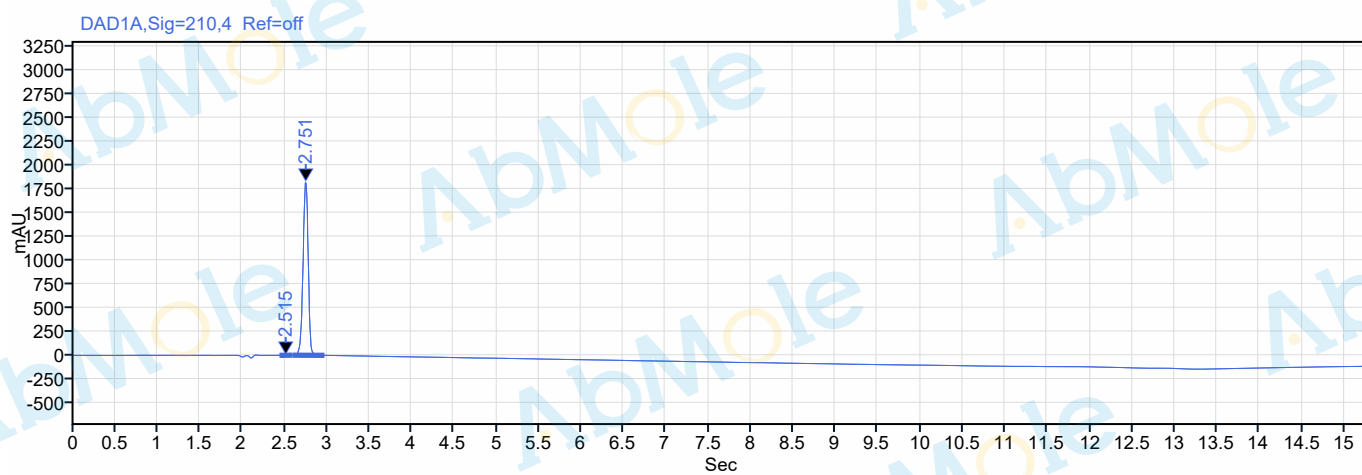

Signal: DAD1A,Sig=210,4 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
2.515		22.8	5.5	0.294
2.751		7733.2	1827.3	99.706