



Agilent Technologies

Sample name: M10382-PROTAC SGK3 degrader-1-01

Injection date:

Instrument: A012

Location:

Inj. volume: 2


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

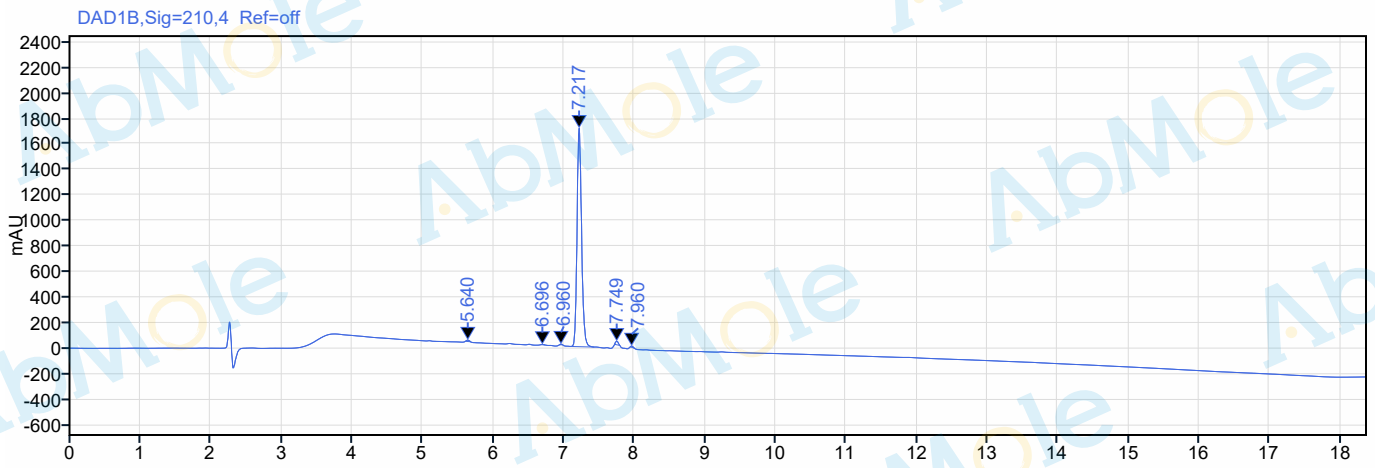

Signal: DAD1B,Sig=210,4 Ref=off

| RT [min] | Area    | Height  | Area% |
|----------|---------|---------|-------|
| 5.640    | 28.05   | 10.81   | 0.36  |
| 6.696    | 4.66    | 2.25    | 0.06  |
| 6.960    | 8.62    | 5.12    | 0.11  |
| 7.217    | 7688.02 | 1710.95 | 98.29 |
| 7.749    | 70.87   | 27.34   | 0.91  |
| 7.960    | 21.60   | 9.89    | 0.28  |