



Agilent Technologies

Sample name: M10589-RGX-104-01

Instrument: A010

Inj. volume: 4

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

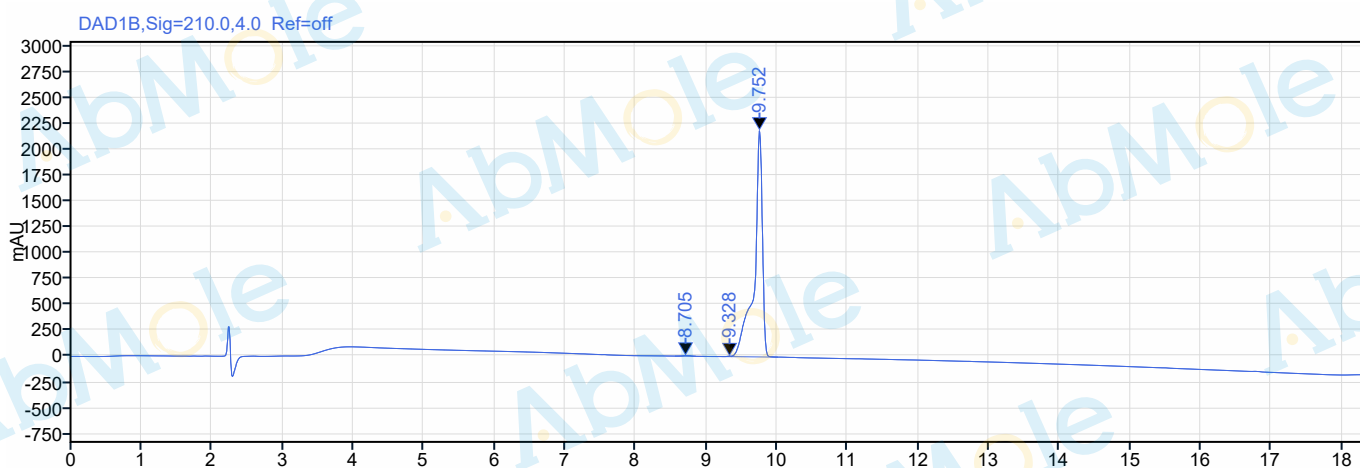

Signal: DAD1B, Sig=210.0, 4.0 Ref=off

RT [min]	Area	Height	Area%
8.705	47.93	5.92	0.27
9.328	16.30	4.98	0.09
9.752	17650.82	2194.19	99.64