


```

=====
Acq. Operator   : admin
Sample Operator : M10593-MRTX1133-01
Acq. Instrument : 3
Location       : P1-B-05
Inj            : 1
Inj Volume     : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.500 µl
=====

```

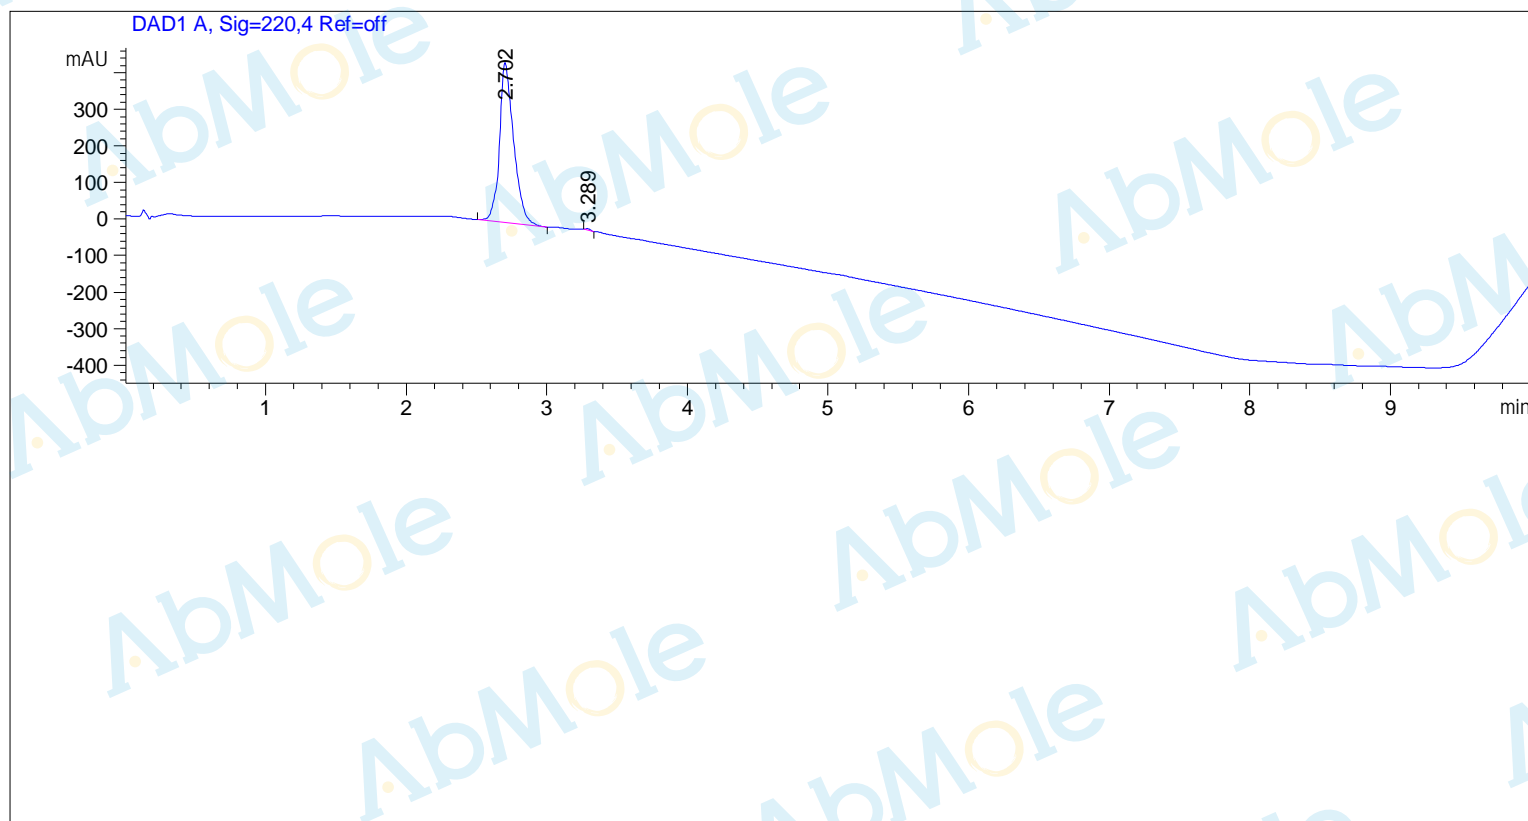

=====
Area Percent Report
=====

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.702	BB	0.1015	3054.19141	437.09113	99.6741
2	3.289	BB	0.0399	9.98539	3.89998	0.3259

Totals :

3064.17680 440.99110