


=====  
Acq. Operator : admin  
Sample Operator : M10955-Daridorexant-01  
Acq. Instrument : 3

Location : P1-A-04

Inj : 1

Inj Volume : 0.100 µl

Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl

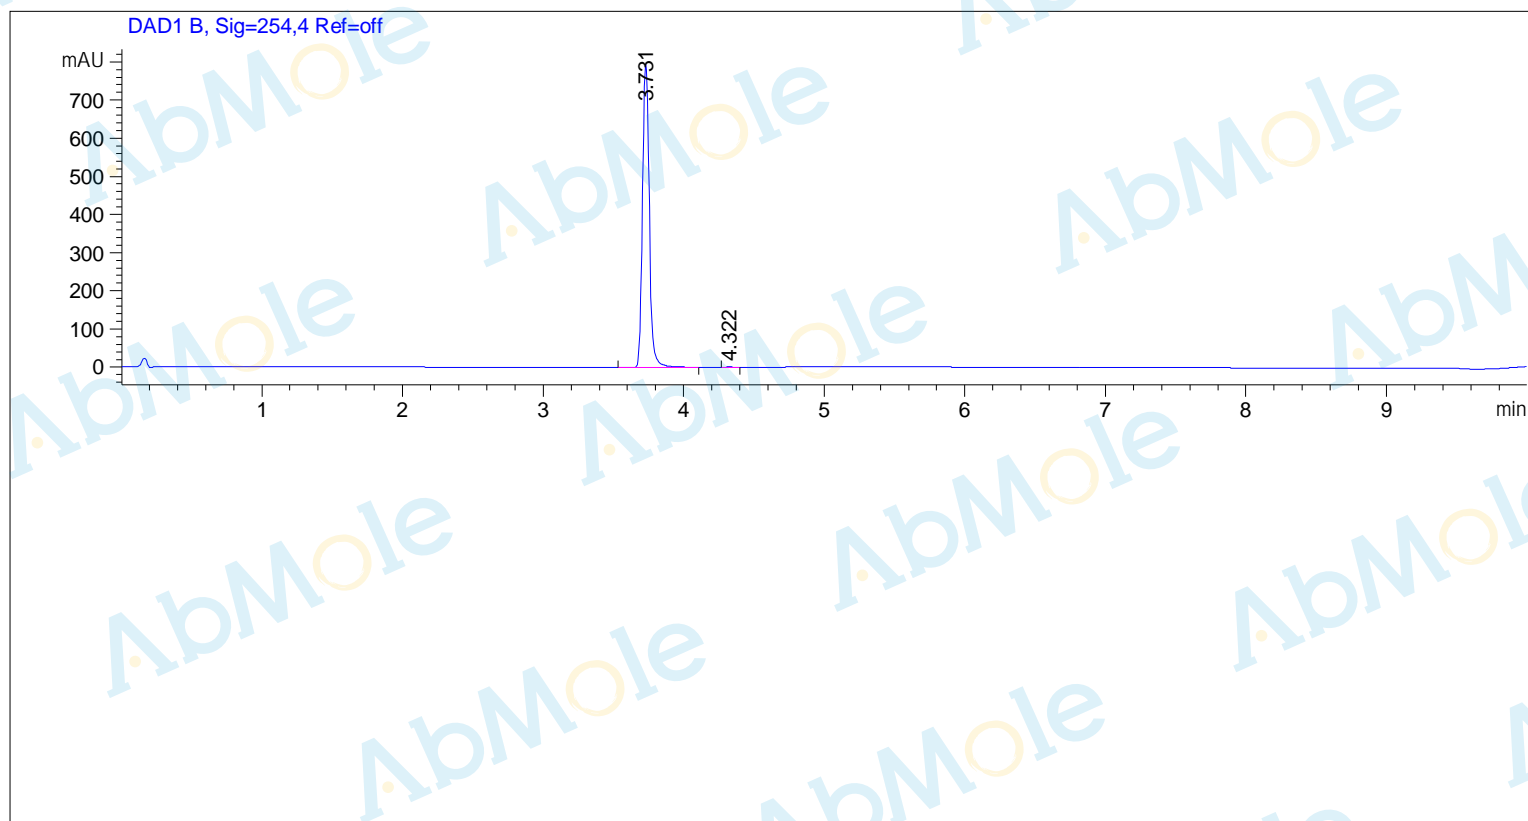

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.731	BB	0.0510	2665.11670	798.05750	99.9237
2	4.322	MM	0.0685	2.03544	4.95476e-1	0.0763

Totals : 2667.15214 798.55297