



Agilent Technologies

Sample name: M11538-MDL-800-01

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

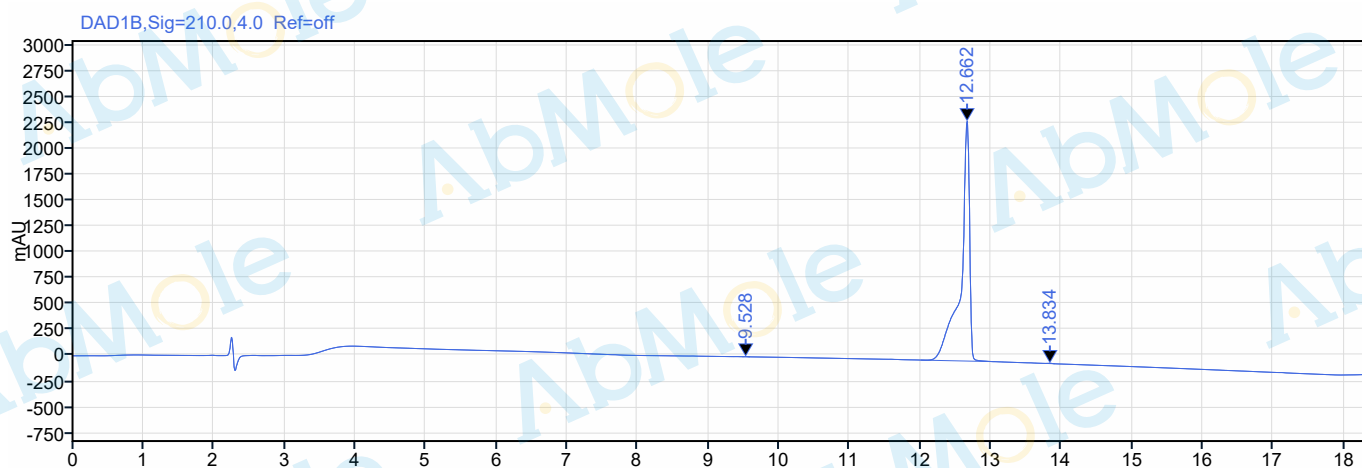

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
9.528	4.97	1.44	0.02
12.662	20067.77	2321.38	99.93
13.834	10.05	2.56	0.05