


Data file: C:\CHEM32\1\DATA\210301\Final.D
 Sample name: M1261-NFAT Inhibitor-01
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 19-29% B in 20min, Flow rate: 1ml/min
 Column: Unitary C18, 4.6*150mm, 5um 100A
 Instrument: Agilent HPLC 1100

Instrument: 1100
 Injection date: 2021/3/1 10:41:27
 Last changed: 2021/3/1 12:23:03
 Location: 14
 Injection: 1 of 1
 Injection volume: 10.000
 Acq. operator: qc

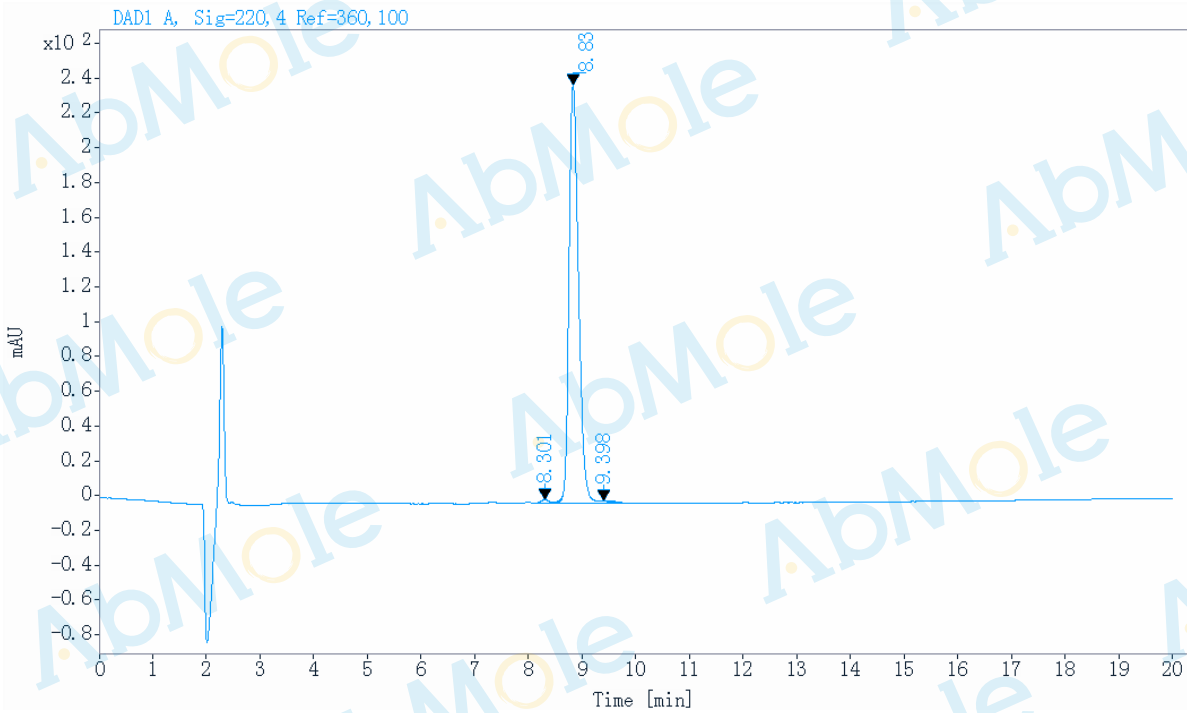

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
8.301	BV E	0.1943	25.3147	1.7545	0.8440
8.830	VV R	0.1900	2970.0847	240.5509	99.0257
9.398	VB E	0.2785	3.9074	0.1698	0.1303
Sum			2999.3068		