


```

=====
Acq. Operator   : SYSTEM                               Seq. Line :    3
Acq. Instrument : 0                                   Location  : P2-E-05
Sample Name     : M13341-VTP50469-01                 Inj       :    1
                                                    Inj Volume: 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl
=====

```

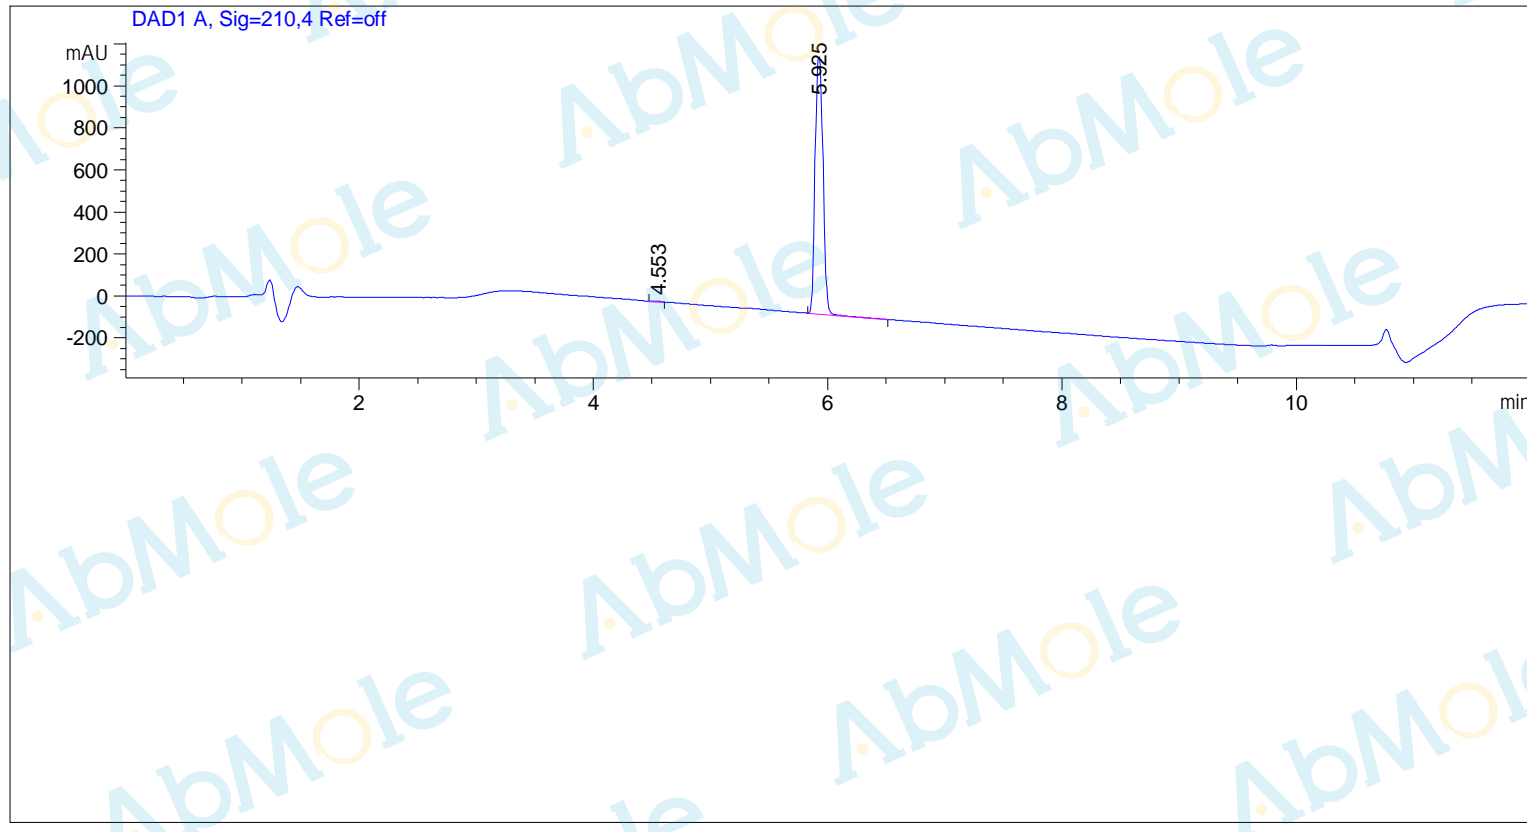

```

=====
                          Area Percent Report
=====

```

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution      :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.553	MM	0.0871	20.80007	3.97971	0.3609
2	5.925	BB	0.0768	5742.86377	1222.73743	99.6391

```
Totals :                5763.66384 1226.71714
```