


=====
Acq. Operator : SYSTEM
Acq. Instrument : 0
Sample Name : M13435-CFT8634-01

Seq. Line : 2
Location : P2-B-02
Inj : 1
Inj Volume : 1.000 µl

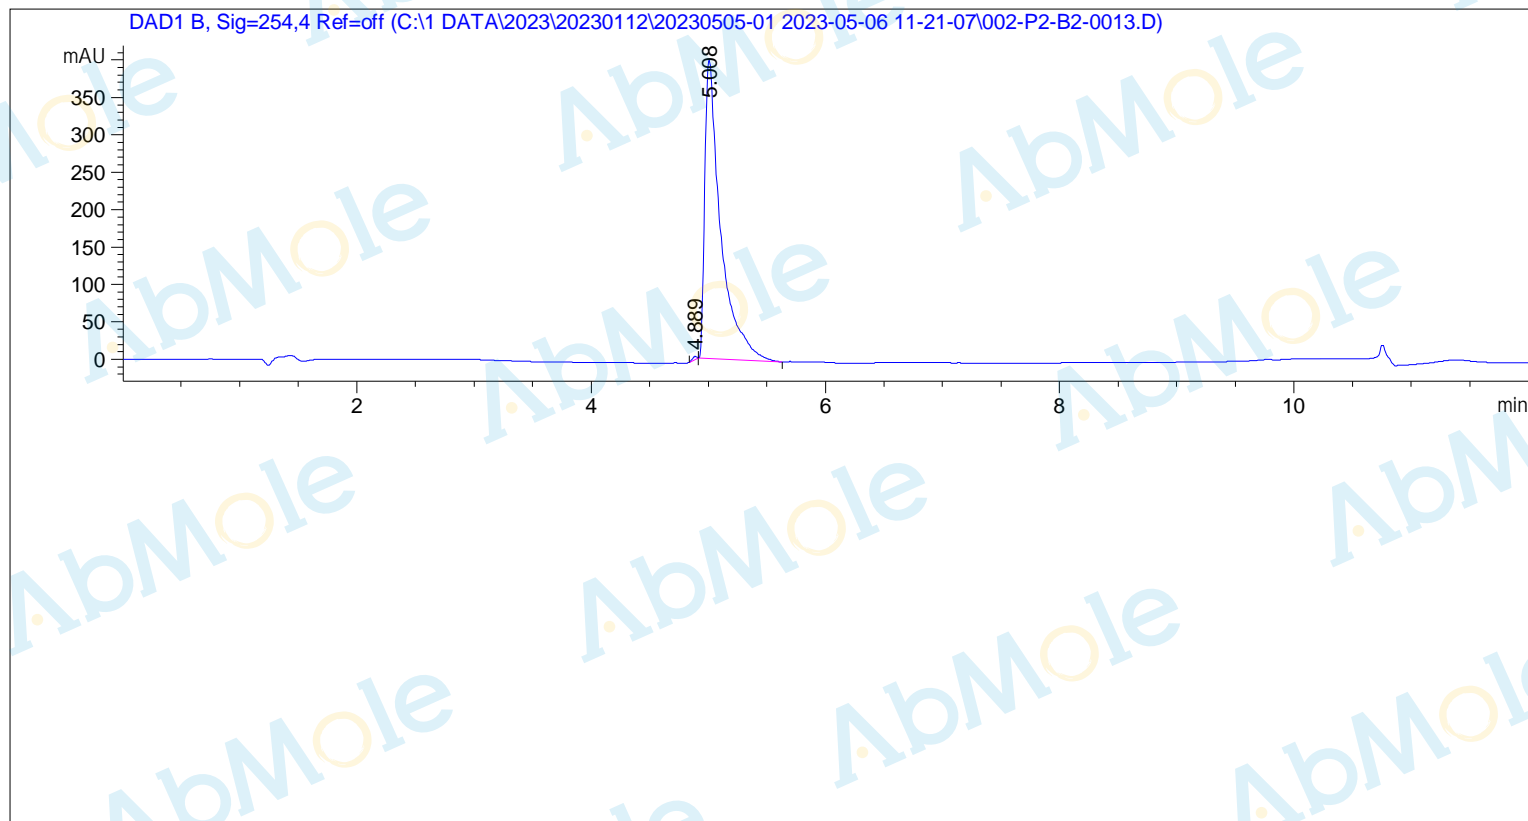

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.889	BB	0.0465	11.76624	4.22263	0.3108
2	5.008	BB	0.1345	3773.83716	398.58298	99.6892

Totals : 3785.60340 402.80560