


```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    1
Acq. Instrument : 0                          Location  : P2-B-01
Sample Name    : M13618-XL413 hydrochloride-01 Inj      :    1
                                                    Inj Volume: 1.000 µl
=====

```

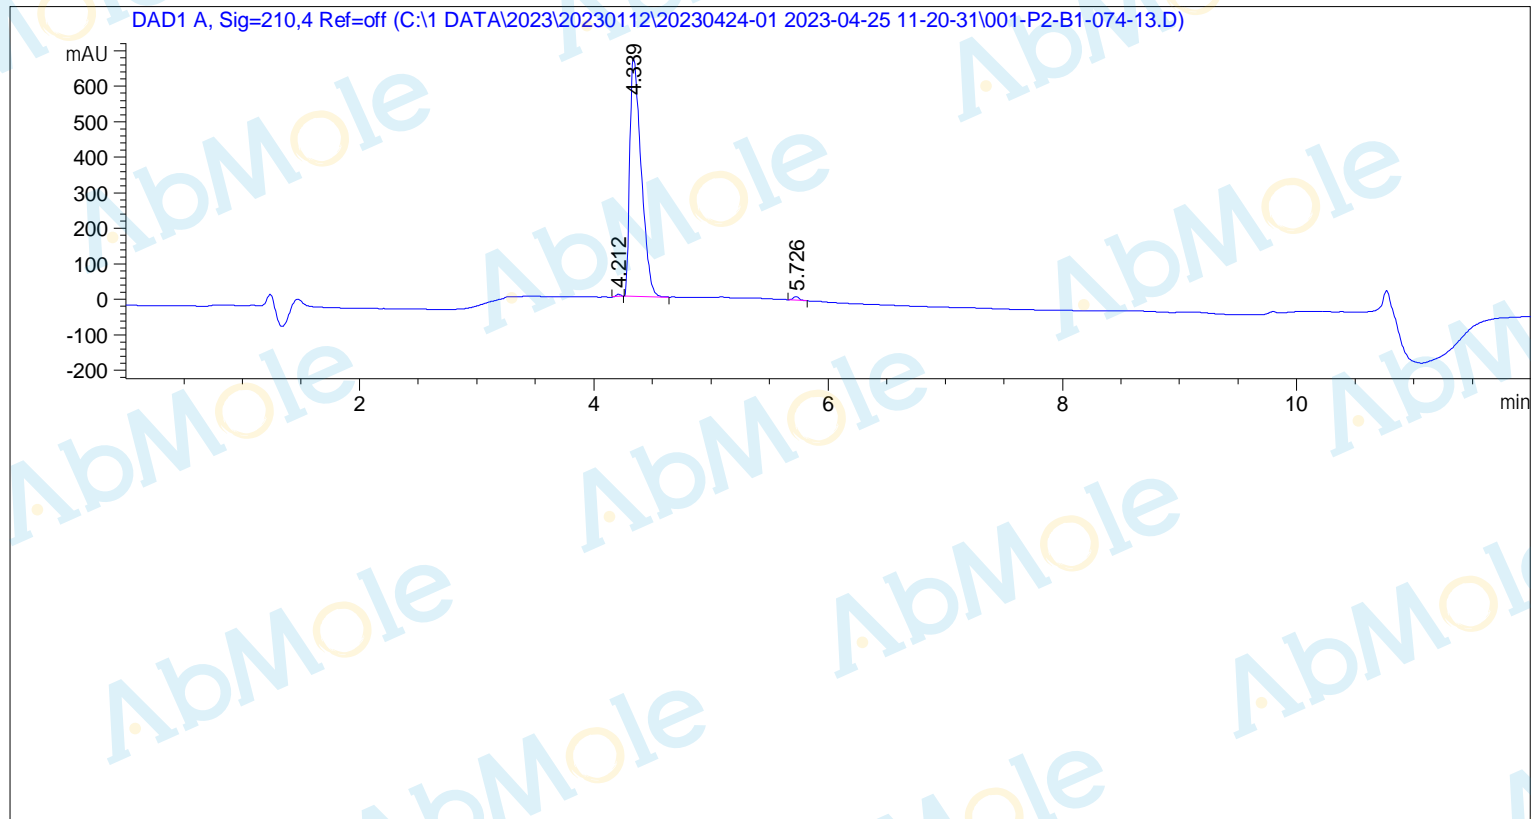

```

=====
                          Area Percent Report
=====

```

```

Sorted By           : Signal
Multiplier          : 1.0000
Dilution            : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.212	BB	0.0454	18.62614	6.92215	0.4044
2	4.339	BB	0.1009	4552.77783	672.90570	98.8544
3	5.726	BB	0.0520	34.13506	9.94809	0.7412

```
Totals :                      4605.53904  689.77593
```