



Agilent Technologies

Sample name: M14647-AA147-02

Instrument: A010

Inj. volume: 1.5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

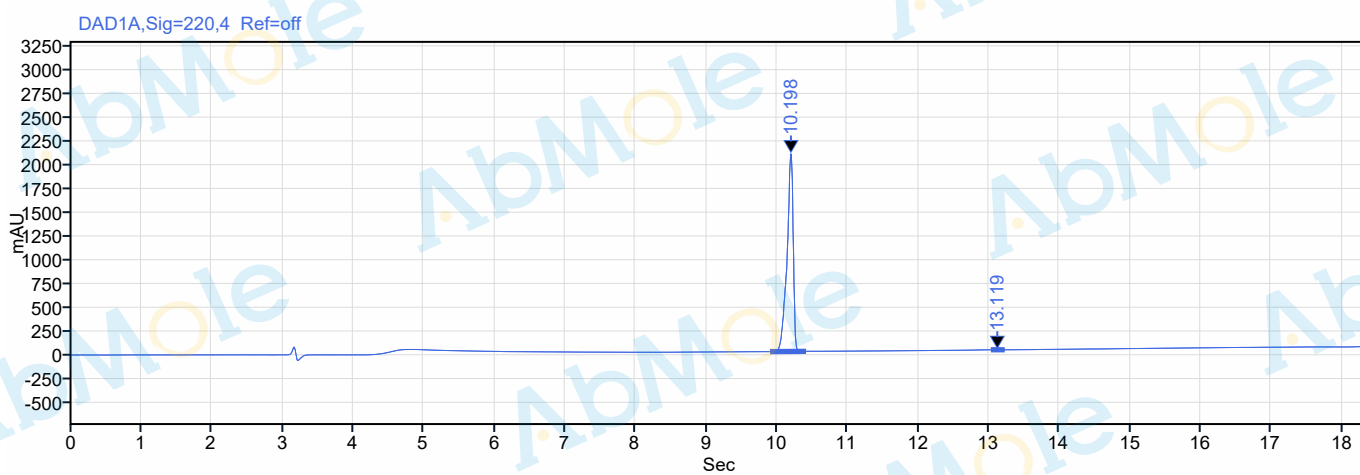

Signal: DAD1A,Sig=220,4 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
10.198		12734.0	2086.6	99.721
13.119		35.6	7.9	0.279