



Agilent Technologies

Sample name: M1556-Hesperitin-02

Instrument: A010

Inj. volume: 4

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

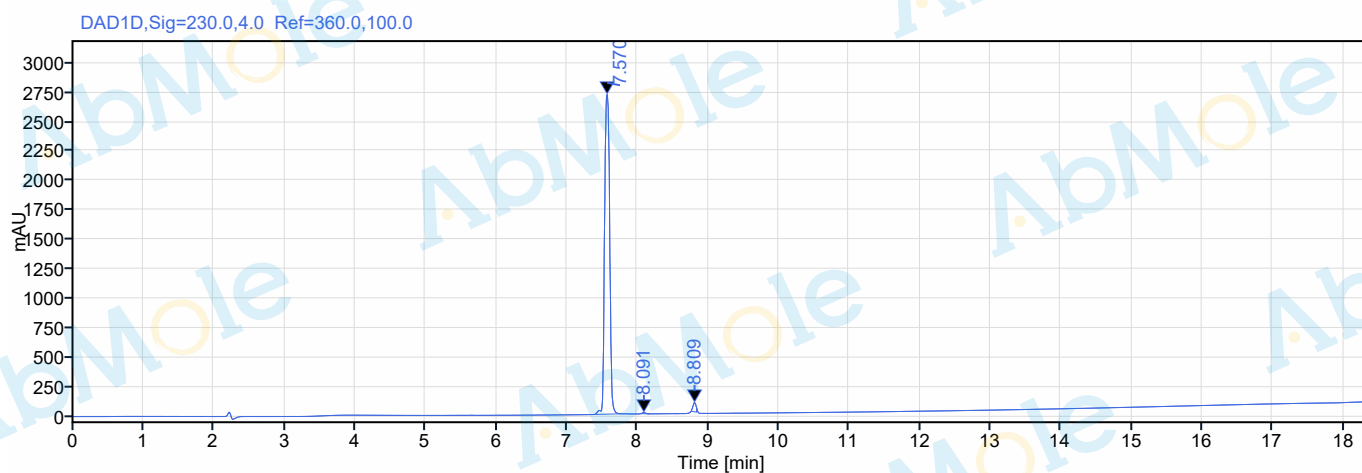

Signal: DAD1D,Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
7.570	MM m	0.40	13551.55	2713.91	98.13
8.091	MB m	0.12	28.97	9.46	0.21
8.809	MM m	0.08	229.62	77.72	1.66