


=====
Acq. Operator : admin
Sample Operator : M1637-ABT-263-14
Acq. Instrument : 3

Location : P2-B-05
Inj : 1
Inj Volume : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl

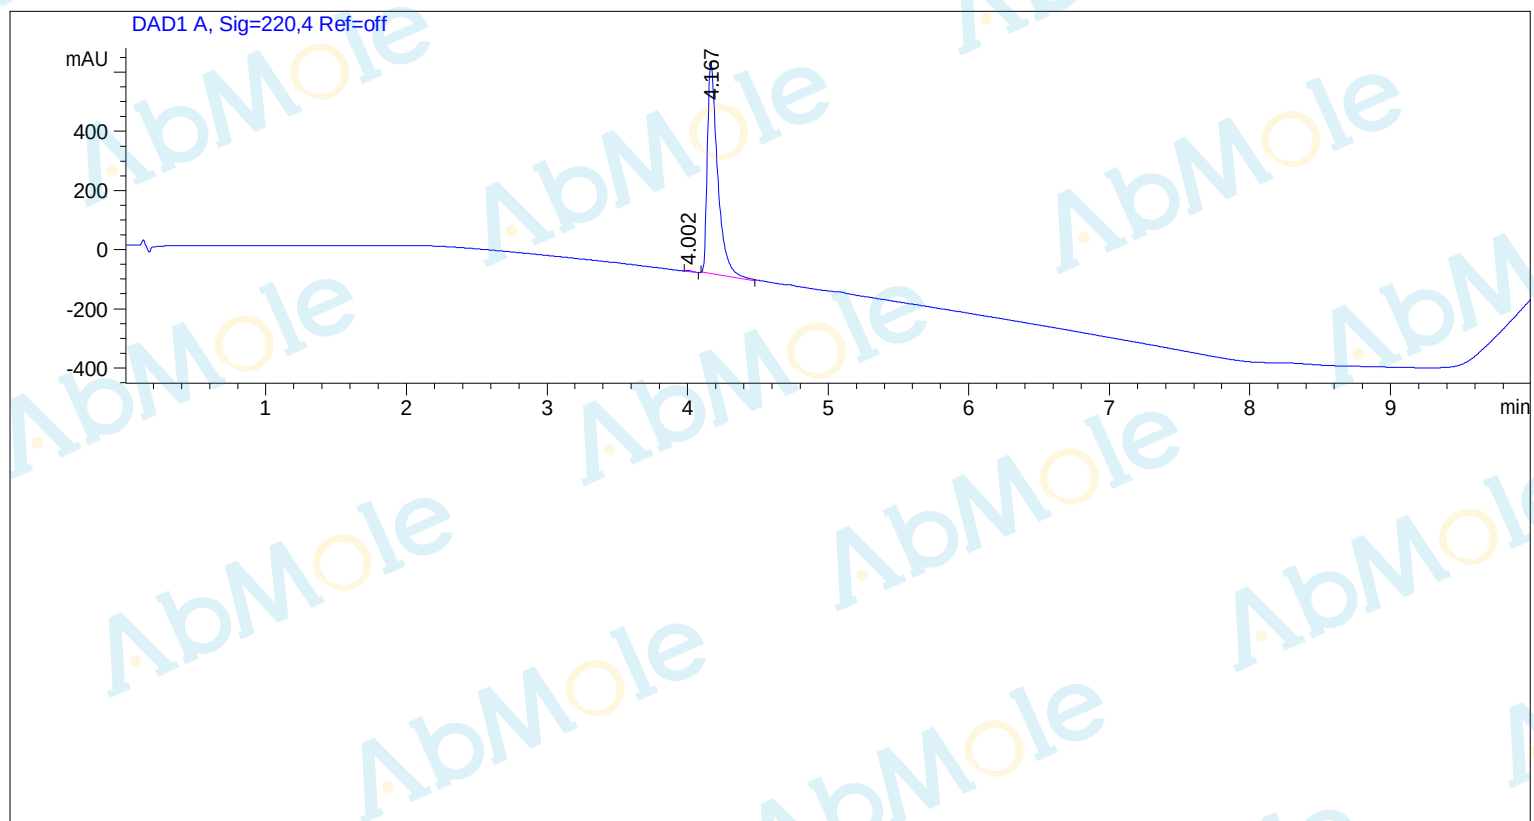

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.002	BB	0.0487	7.41978	2.49718	0.2047
2	4.167	MM	0.0841	3616.53760	717.01758	99.7953

Totals :

3623.95737 719.51476