




Sample name: M1642-ABT-751-01
Instrument: A010
Inj. volume: 2
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

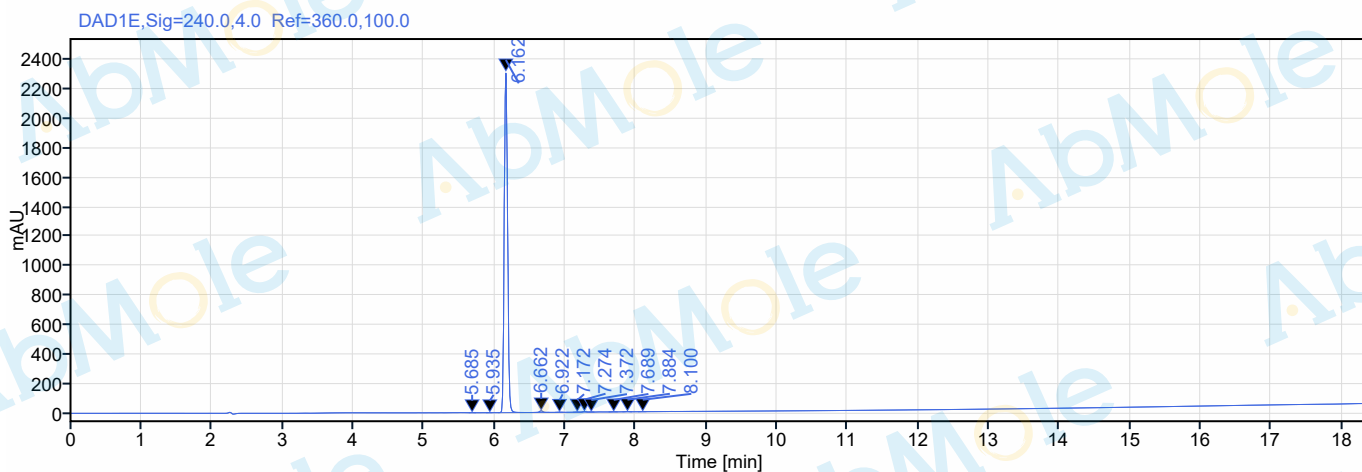

Signal: DAD1E, Sig=240.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
5.685	MM m	0.10	1.73	0.62	0.02
5.935	MM m	0.09	0.45	0.18	0.01
6.162	BB	0.41	7765.02	2319.51	99.17
6.662	MB m	0.22	35.30	11.00	0.45
6.922	BB	0.11	3.30	1.12	0.04
7.172	MM m	0.10	2.85	0.99	0.04
7.274	BB	0.12	11.62	3.75	0.15
7.372	MM m	0.08	1.15	0.48	0.01
7.689	MM m	0.13	2.67	0.68	0.03
7.884	MB m	0.14	5.01	1.40	0.06
8.100	MM m	0.12	0.79	0.23	0.01