


=====

Acq. Operator	: System	Seq. Line	: 7
Acq. Instrument	: LC1260	Location	: Vial 5
Injection Date	: 10/27/2020 4:07:21 PM	Inj	: 1
		Inj Volume	: 0 µl
Different Inj Volume from Sequence !		Actual Inj Volume	: 1 µl
Acq. Method	: E:\DATA\Data\20201027\20200913-01 2020-10-27 12-32-26\10-90 AD 254 15MIN.M		
Last changed	: 10/27/2020 1:38:20 PM by System		
Analysis Method	: D:\PUBLIC\20201023\DEF_LC 2020-10-23 17-38-03\YZJ-1023-1.D\DA.M (5-95 6MIN.M)		
Last changed	: 10/25/2020 1:04:15 PM		

=====

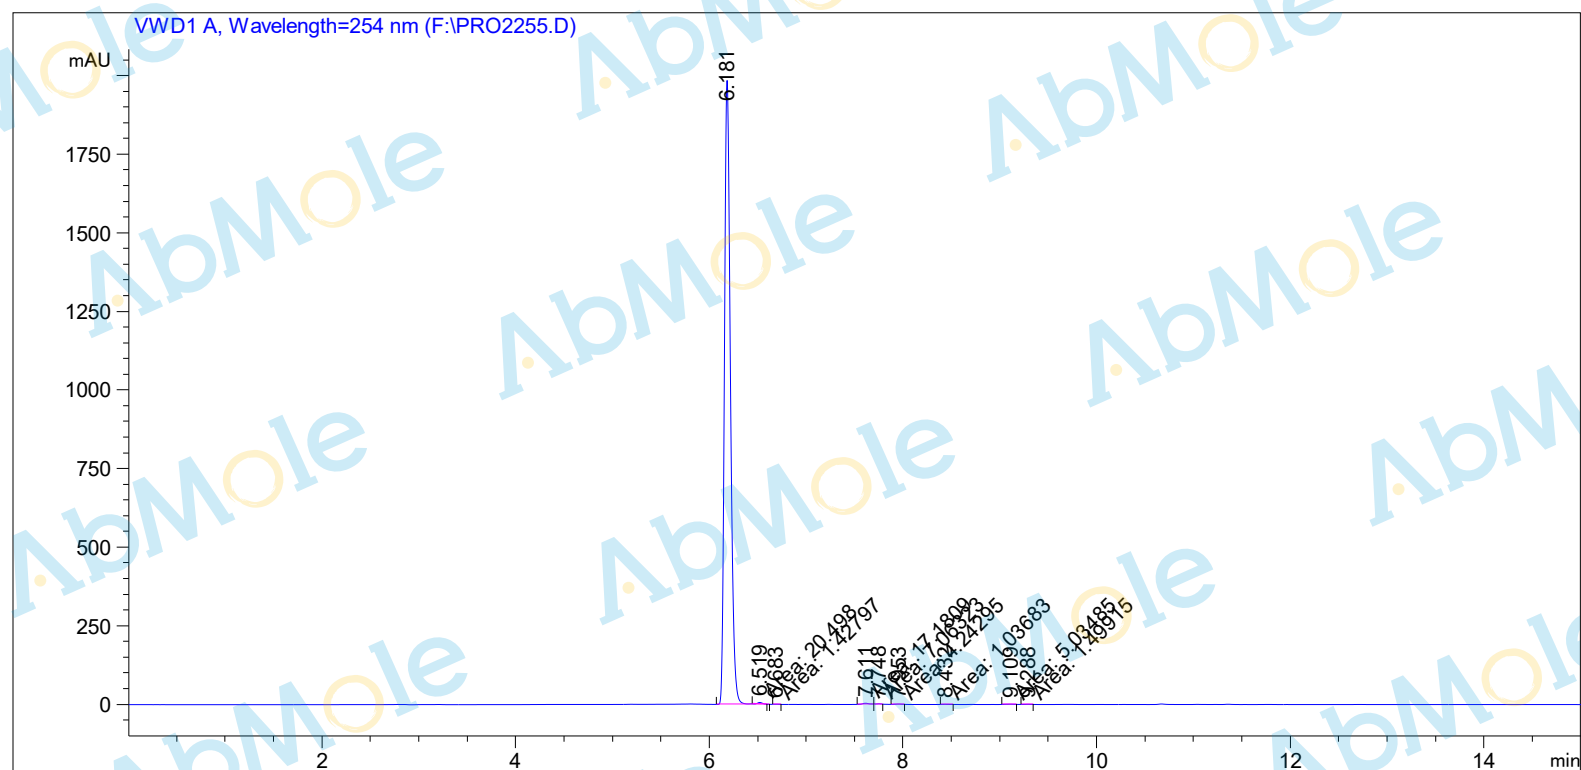

=====

Area Percent Report

=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=254 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.181	MM R	0.0714	8520.10156	1989.04565	99.3240
2	6.519	MM T	0.0715	20.49799	5.41353	0.2390
3	6.683	MM	0.0511	1.42797	4.65495e-1	0.0166
4	7.611	MF	0.0841	17.18087	3.40396	0.2003

Sample Name: BKM120-02

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
5	7.748	FM	0.0704	7.06323	1.67114	0.0823
6	7.953	MM	0.0684	4.24295	1.03400	0.0495
7	8.432	MM	0.0714	1.03683	2.41872e-1	0.0121
8	9.109	MM	0.0943	5.03485	8.89910e-1	0.0587
9	9.288	MM	0.0783	1.49915	3.19166e-1	0.0175

Totals : 8578.08540 2002.48472

*** End of Report ***