



Agilent Technologies

Sample name: M1704-Enzastaurin-01

Instrument: A012

Inj. volume: 3

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

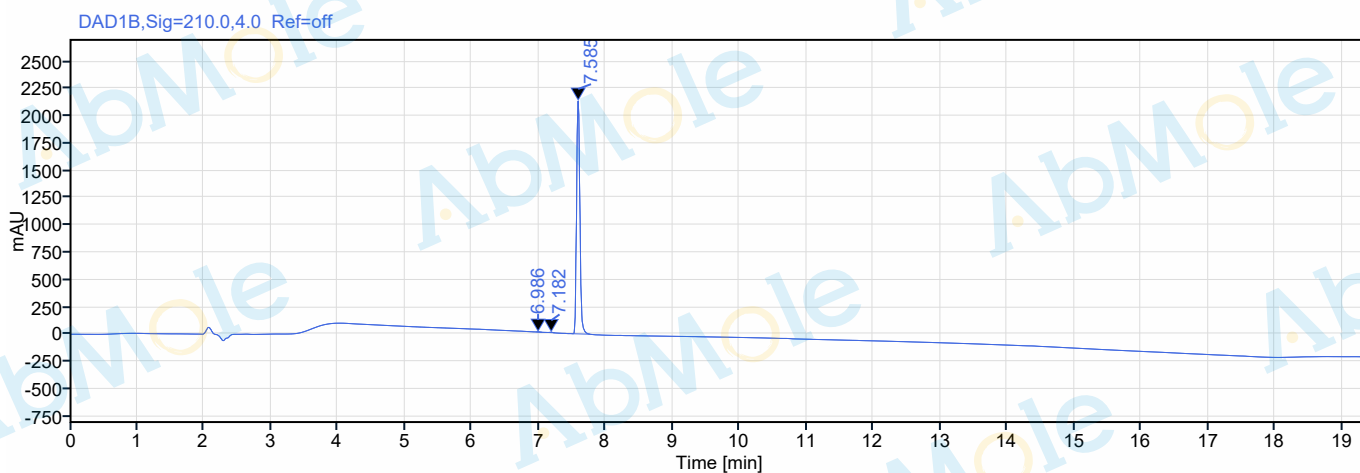

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
6.986	3.70	1.18	0.05
7.182	10.63	3.54	0.15
7.585	7218.58	2133.74	99.80