



Agilent Technologies

Sample name: M1715-GDC-0941 (Pictilisib)-05

Injection date:

Instrument: A012

Location:

Inj. volume: 2


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

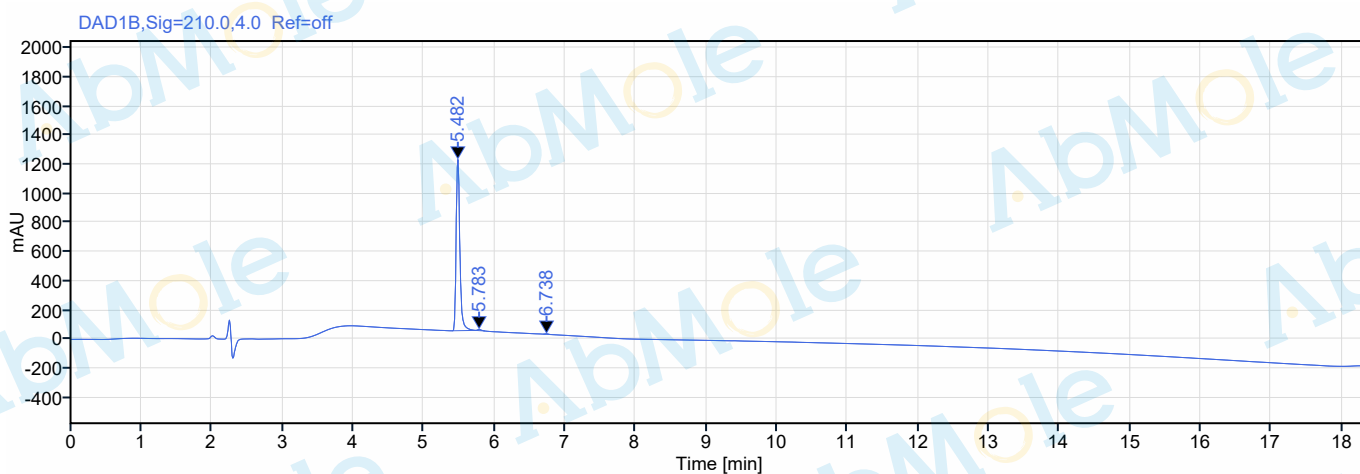

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
5.482	4289.86	1174.95	99.12
5.783	28.55	7.91	0.66
6.738	9.62	3.28	0.22