



Sample name: M1743-X-376-02

Instrument: A010

Inj. volume: 1

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

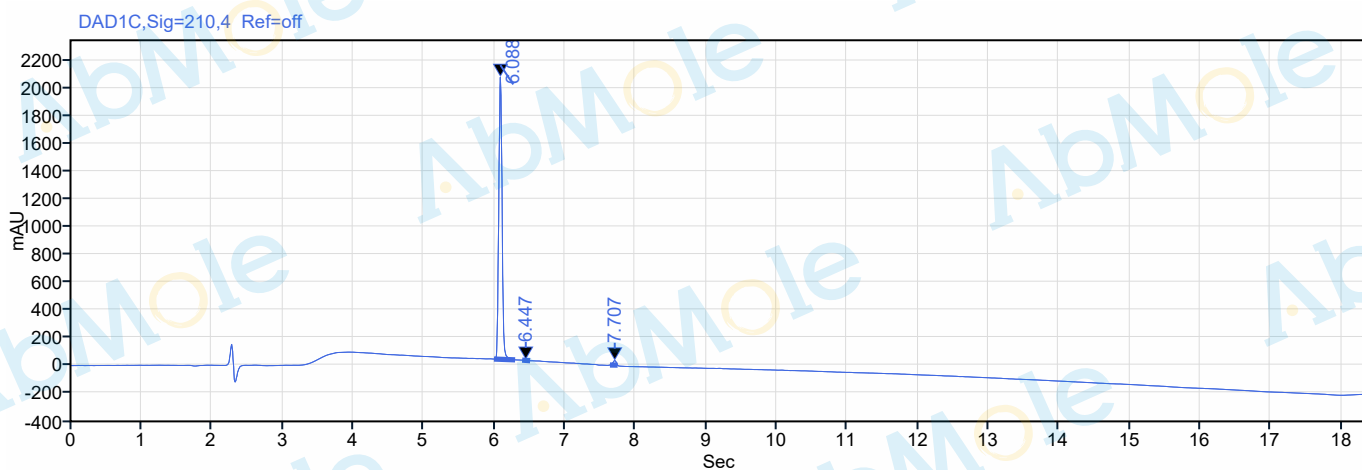

Signal: DAD1C,Sig=210,4 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
6.088		0.30	6675.9	2037.3	98.28
6.447		0.11	13.9	4.4	0.21
7.707		0.11	102.7	32.7	1.51