



Agilent Technologies

Sample name: M1754-WP1130-01

Instrument: A012

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

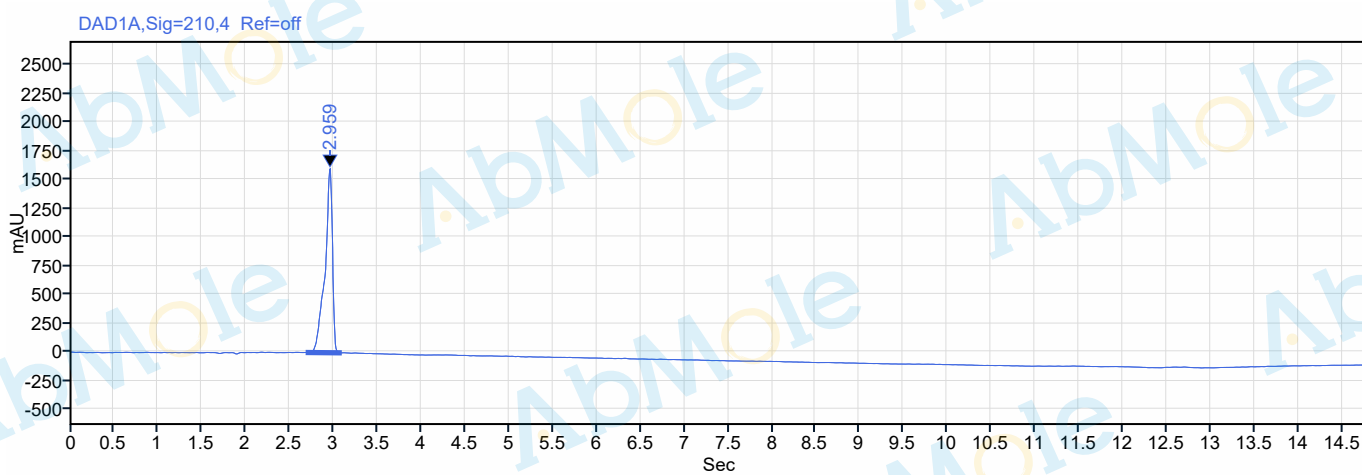

Signal: DAD1A,Sig=210,4 Ref=off

| RT [min] | Peak<br>Resolution<br>USP | Area   | Height | Area%   |
|----------|---------------------------|--------|--------|---------|
| 2.959    |                           | 9530.8 | 1608.3 | 100.000 |