



Agilent Technologies

Sample name: M1837-MK-2206 2HCI-08-1

Instrument: A010

Inj. volume: 1

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

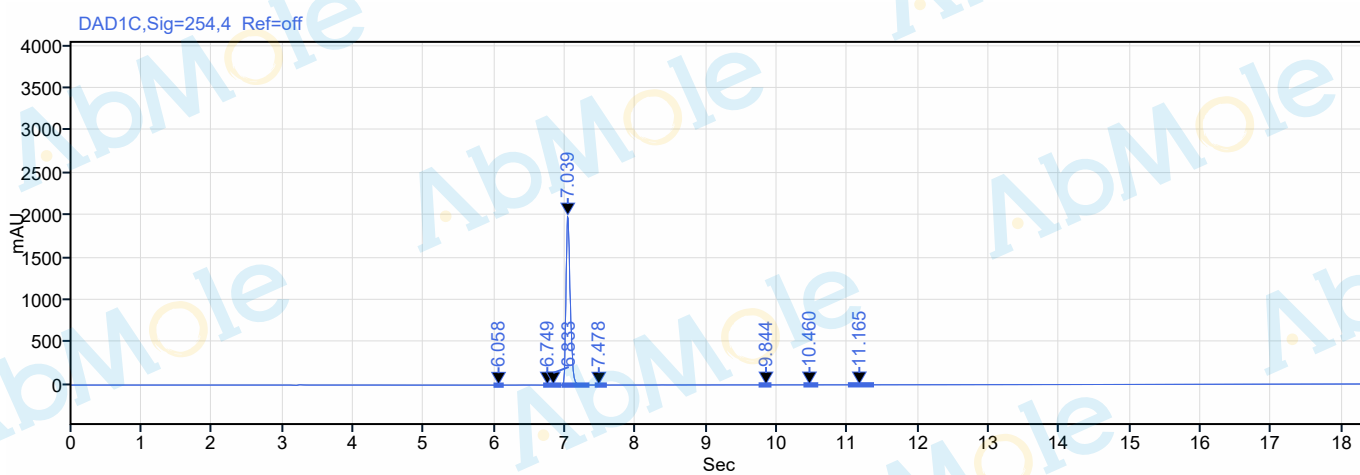

Signal: DAD1C,Sig=254,4 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
6.058		0.14	2.5	0.8	0.03
6.749		0.10	4.6	1.7	0.05
6.833		0.16	9.8	2.8	0.12
7.039		0.40	8381.4	1996.8	99.59
7.478		0.17	3.5	0.8	0.04
9.844		0.18	3.7	0.9	0.04
10.460		0.21	3.6	0.8	0.04
11.165		0.37	6.8	0.7	0.08