




Agilent Technologies

Sample name: M1839-MDV3100-05
Instrument: 1
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

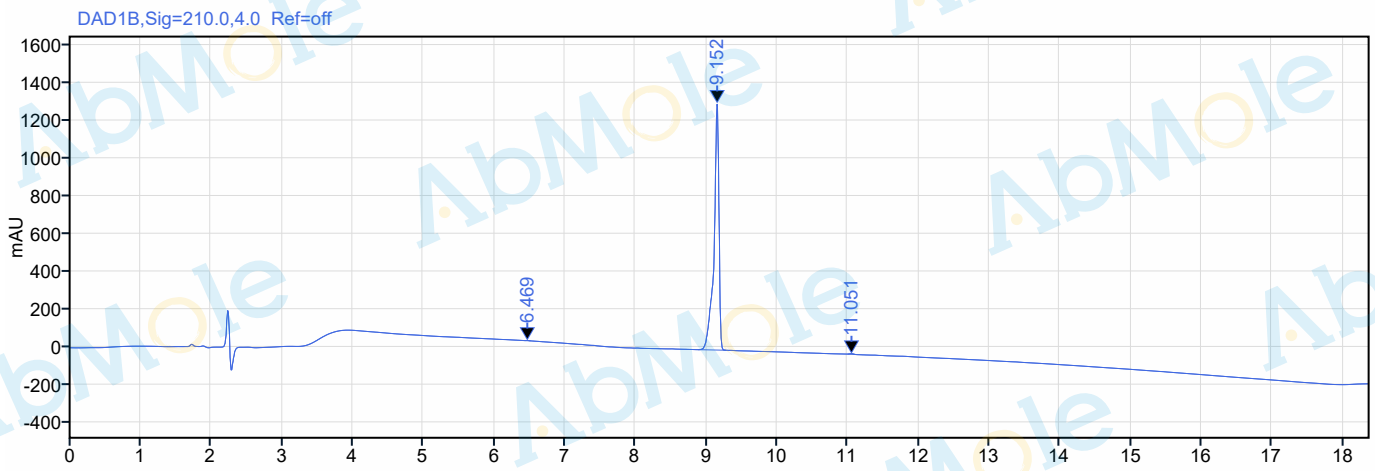

Signal: DAD1B, Sig=210.0, 4.0 Ref=off

RT [min]	Area	Height	Area%
6.469	3.03	1.05	0.05
9.152	6374.29	1306.74	99.79
11.051	10.45	3.07	0.16
Sum	6387.76		