



Agilent Technologies

Sample name: M2022-Torin 2-02

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

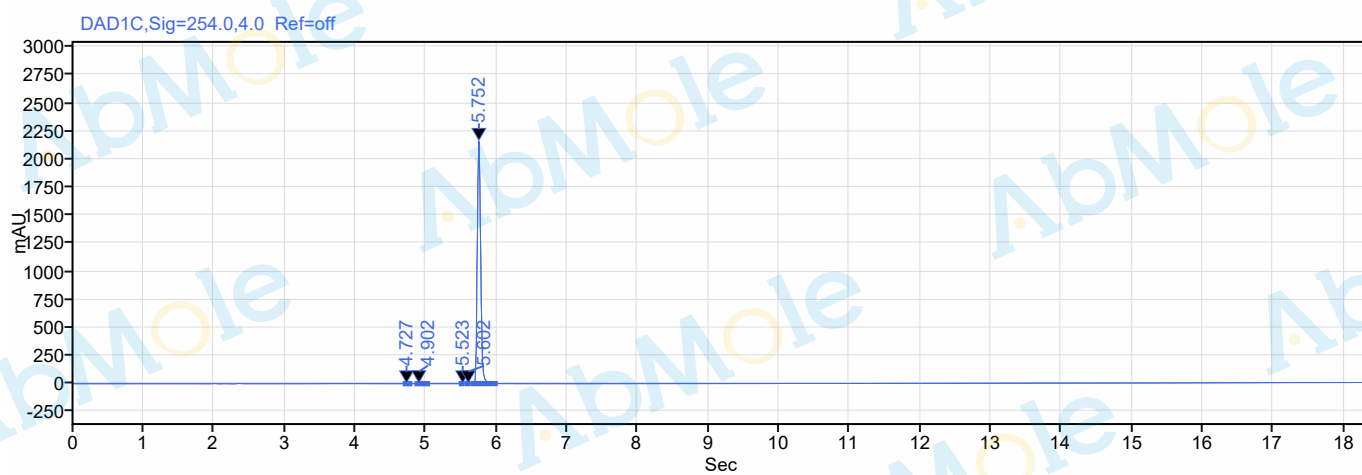

Signal: DAD1C,Sig=254.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
4.727		0.14	1.9	0.5	0.03
4.902		0.22	6.3	1.8	0.09
5.523		0.08	0.3	0.1	0.00
5.602		0.09	0.8	0.3	0.01
5.752		0.38	7229.5	2163.0	99.87