


```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    2
Acq. Instrument : 0                          Location  : P2-A-07
Sample Name    : M2059-A-922500-02-1         Inj       :    1
                                                Inj Volume: 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl
=====

```

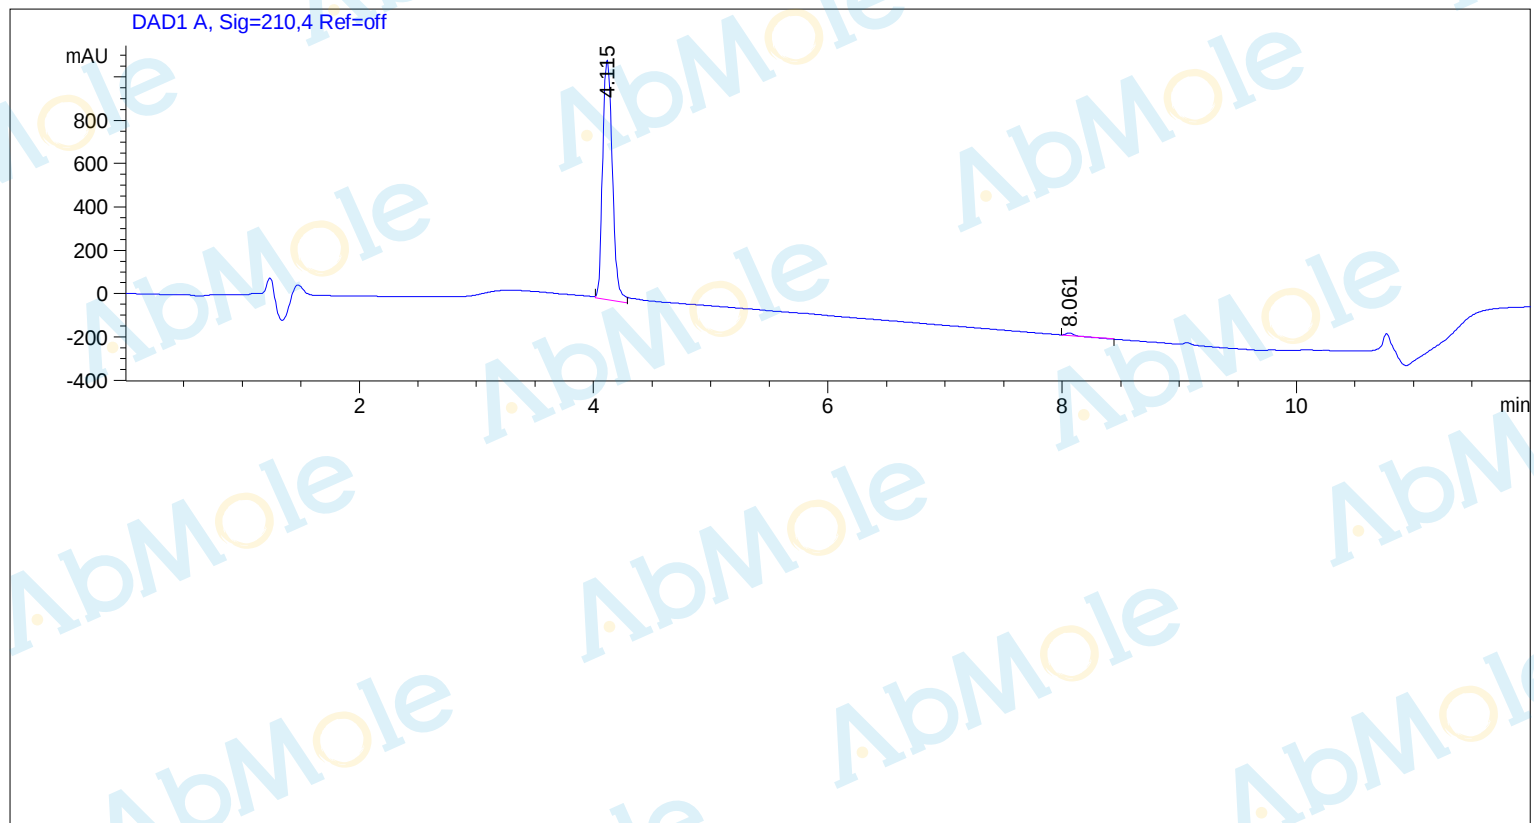

```

=====
                          Area Percent Report
=====

```

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.115	MM	0.0964	6407.04395	1108.19202	99.1490
2	8.061	BB	0.0681	54.99379	12.31139	0.8510

Totals : 6462.03773 1120.50340