




Sample name: M2082-Streptozotocin-10  
Instrument: 2  
Inj. volume: HPLC  
Acq. method:  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

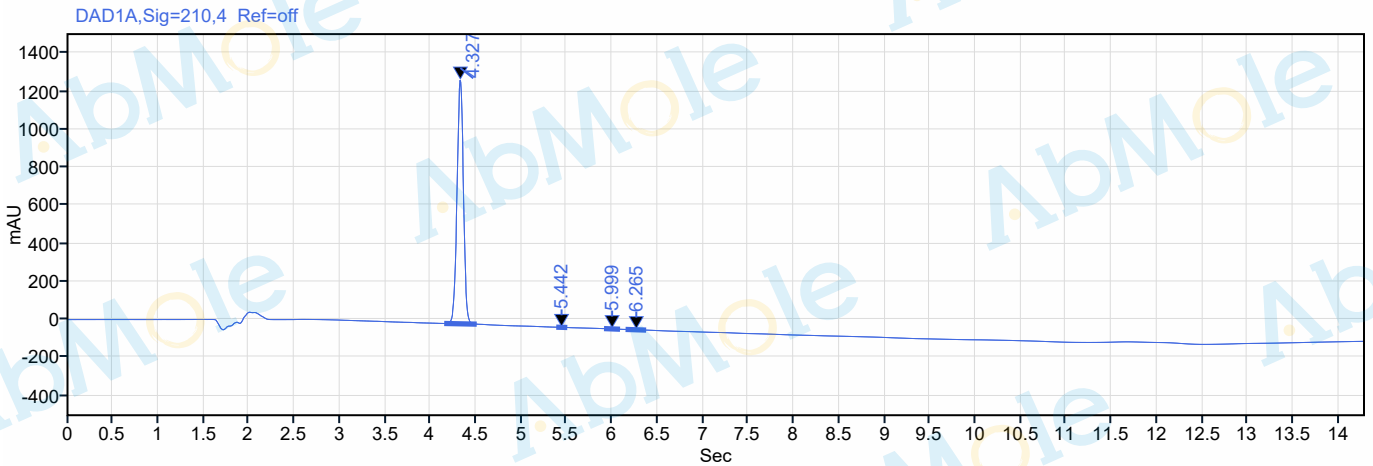

Signal: DAD1A, Sig=210,4 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
4.327		0.08	6313.9	1285.4	99.50
5.442		0.07	4.1	0.9	0.06
5.999		0.09	15.4	2.9	0.24
6.265		0.09	12.5	2.1	0.20
		Sum	6345.91		