



Agilent Technologies

Sample name: M20832-ML-SI3-02

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

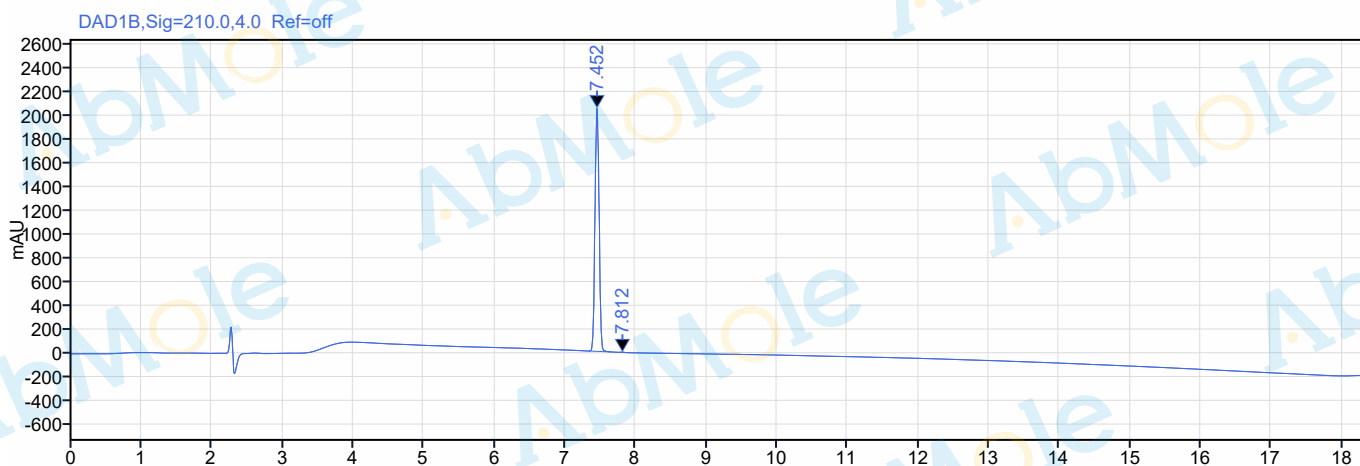

Signal: DAD1B, Sig=210.0, 4.0 Ref=off

RT [min]	Area	Height	Area%
7.452	8336.45	2049.99	99.91
7.812	7.63	2.56	0.09