




Agilent Technologies

Sample name: M21307-Romiplostim-01
Instrument: 1
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

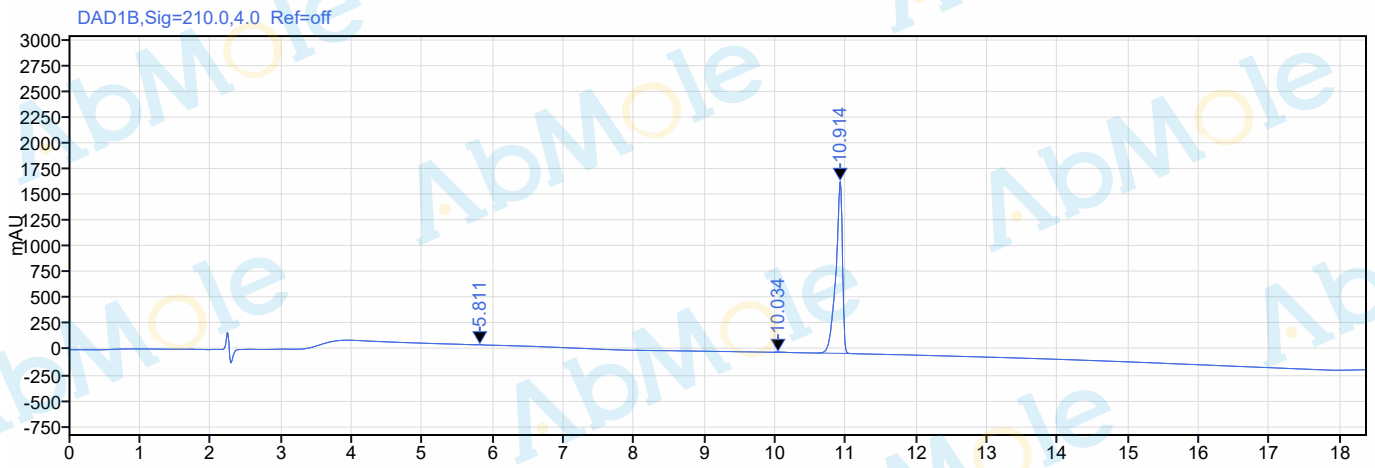

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
5.811	11.84	4.49	0.11
10.034	12.06	2.37	0.11
10.914	10909.98	1673.93	99.78
Sum	10933.89		