



Agilent Technologies

Sample name: M2215-MK-4827 (Niraparib) -04

Injection date:

Instrument: A010

Location:

Inj. volume: 1.5


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

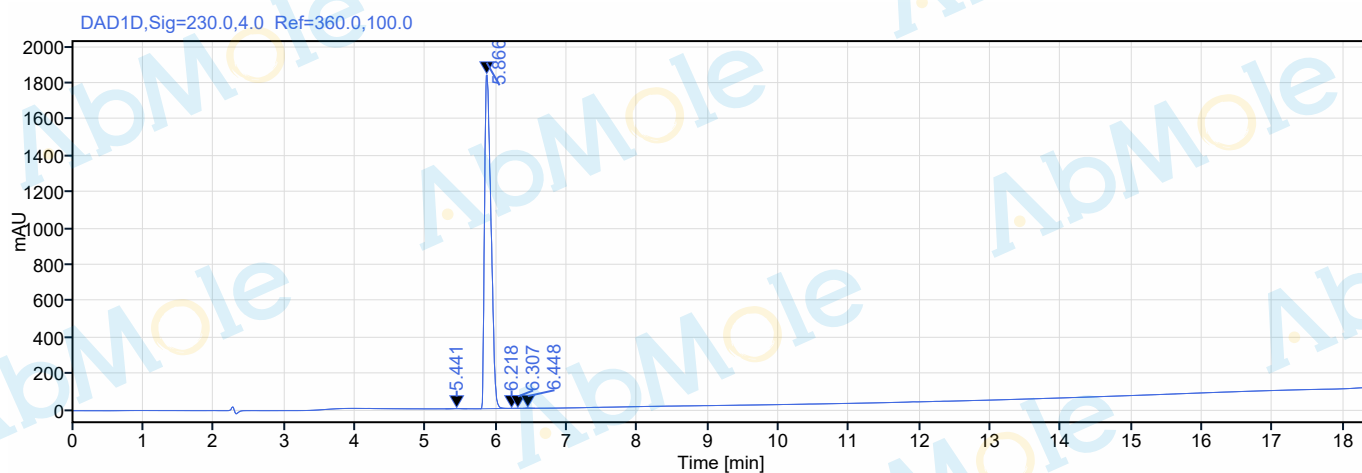

Signal: DAD1D,Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
5.441	MM m	0.31	14.21	1.72	0.12
5.866	BB	0.40	11607.64	1838.32	99.82
6.218	MM m	0.08	0.26	0.13	0.00
6.307	MM m	0.09	0.63	0.20	0.01
6.448	MB m	0.17	6.14	1.69	0.05