



Agilent Technologies

Sample name: M22486-AH-7614-01

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

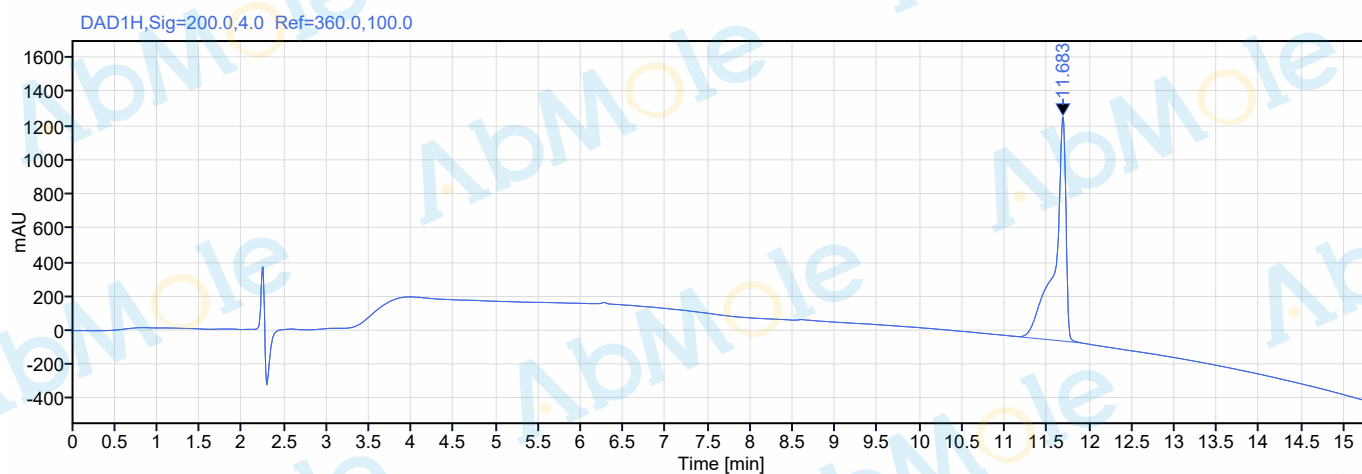

Signal: DAD1H,Sig=200.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
11.683	MM m	0.82	12084.60	1316.07	100.00