



Agilent Technologies

Sample name: M2259-Biapenem-02

Instrument: A012

Inj. volume: 6

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

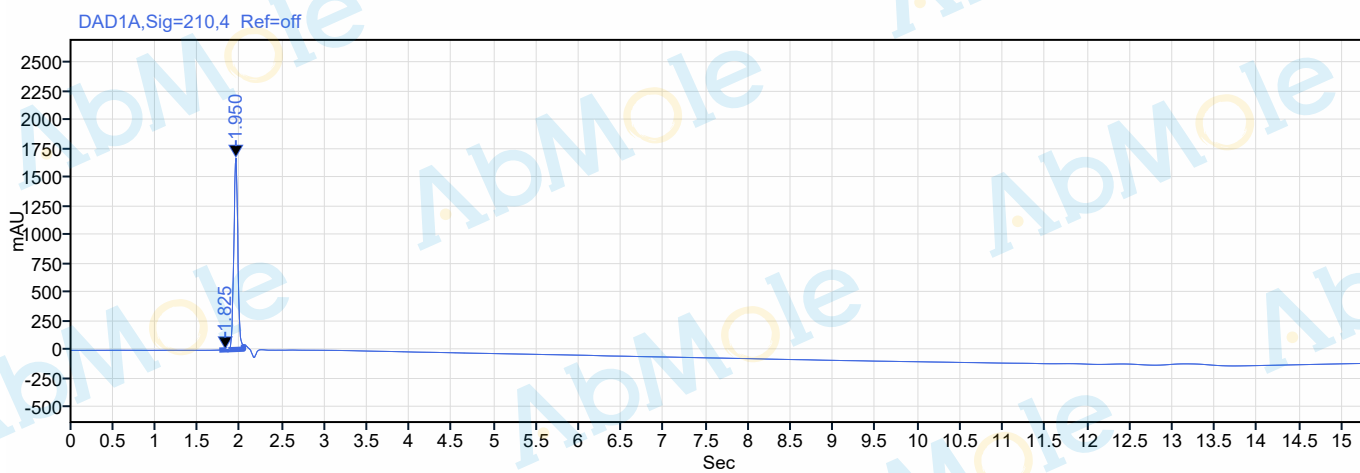

Signal: DAD1A,Sig=210,4 Ref=off

RT [min]	Peak Resolution	Area	Height	Area%
1.825		8.3	2.2	0.149
1.950		5580.4	1665.6	99.851