



File D:\DATA\BATCCD\CGS 21680 hydrochloride-02-LCMS040.D Tgt Mass (EZ):
Sample Name : CGS 21680 hydrochloride-02 Location : P1-B-03
Acq. Operator : BATCCD-P Inj : 0
Spec. Reported : MS Integration Inj Volume : 0.5 ul
Acq. Method : C:\Chem32\1\METHODS\HPLC-A.M
Analysis Method : C:\CHEM32\1\METHODS\HPLC-A.M
Sample Info : Easy-Access Method: 'HPLC-A.M'
Method Info : Column: L-column2 ODS: 150 mm*4.6 mm*5.0 um;
Mobile Phase: A: Water (0.05% TFA) B: ACN (0.05%TFA) ;
Gradient: Pump1:B from 5% to 100% for 10 min and hold 100% for 5.0 min;
Flow Rate: 1.0 mL/min;
Column Temperature: 40

DAD1 B, Sig=214,4 Ref=off

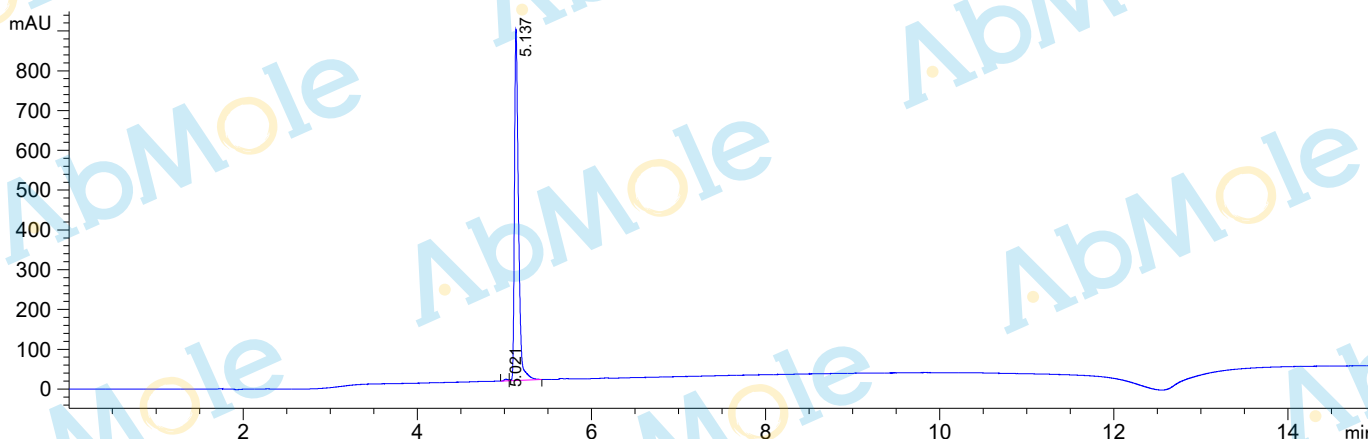

DAD1 A, Sig=254,4 Ref=off

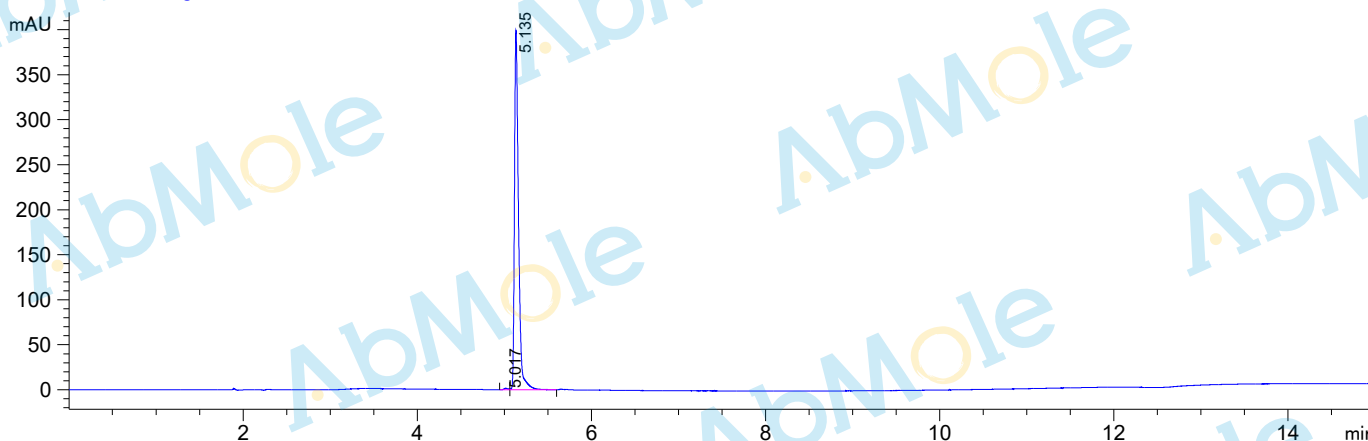

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.02	0.05	12.69	4.20	0.45
5.14	0.05	2828.97	834.71	99.55

Integration Results for DAD1 A, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.02	0.05	5.33	1.67	0.41
5.13	0.05	1291.15	394.84	99.59