


=====  
Acq. Operator : SYSTEM  
Acq. Instrument : 0  
Sample Name : M2288-Carboplatin-06

Seq. Line : 2  
Location : P1-F-02  
Inj : 1  
Inj Volume : 1.000 µl

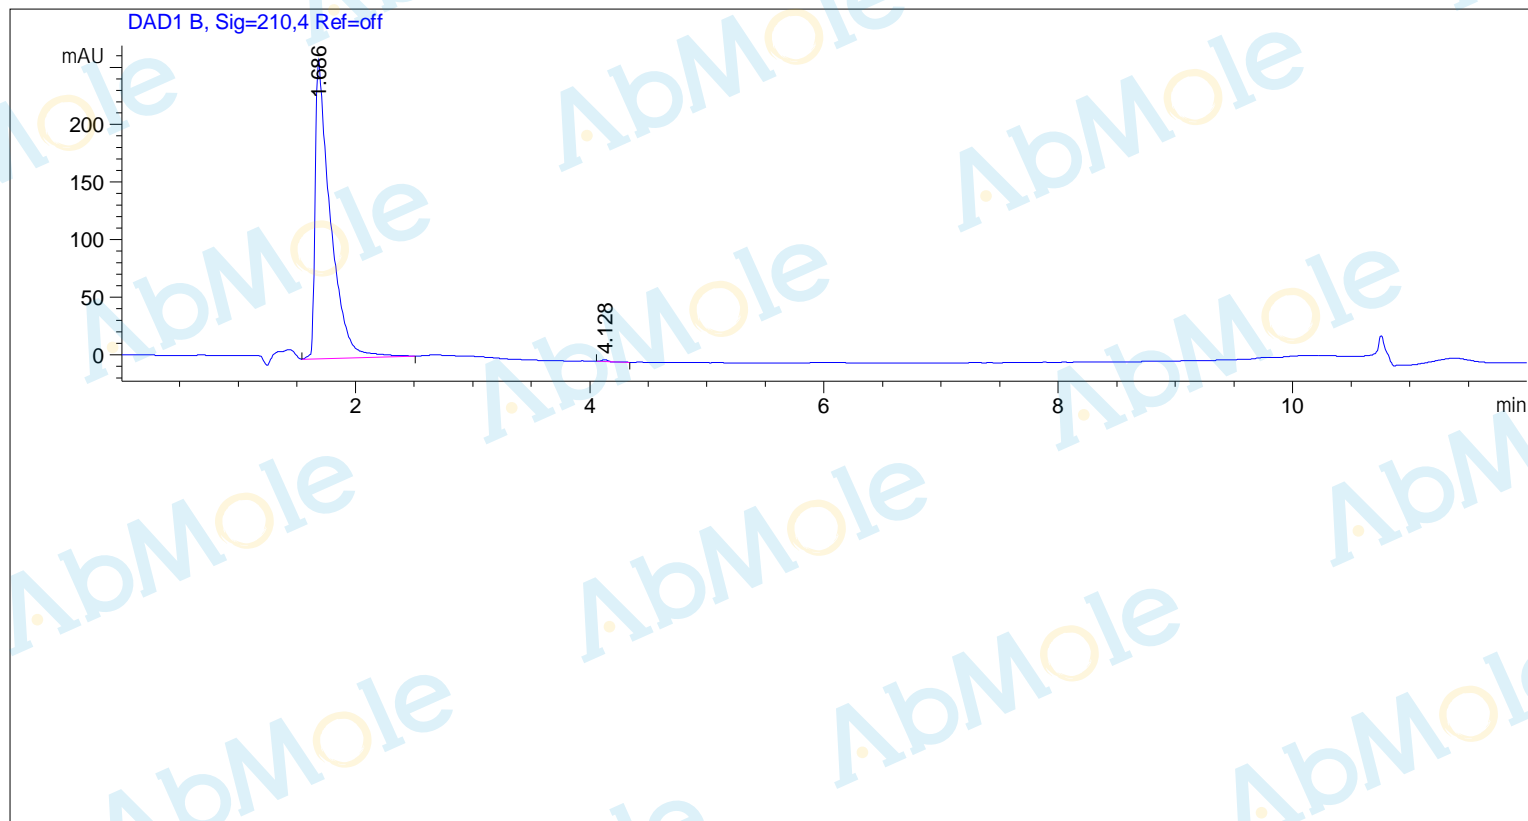

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.686	BB	0.1234	2344.58691	259.47260	99.7535
2	4.128	BB	0.0522	5.79319	1.68121	0.2465

Totals : 2350.38010 261.15380