



Agilent Technologies

Sample name: M2296-3-Methyladenine (3-MA)-09

Injection date:

Instrument: A010

Location:

Inj. volume: 2


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

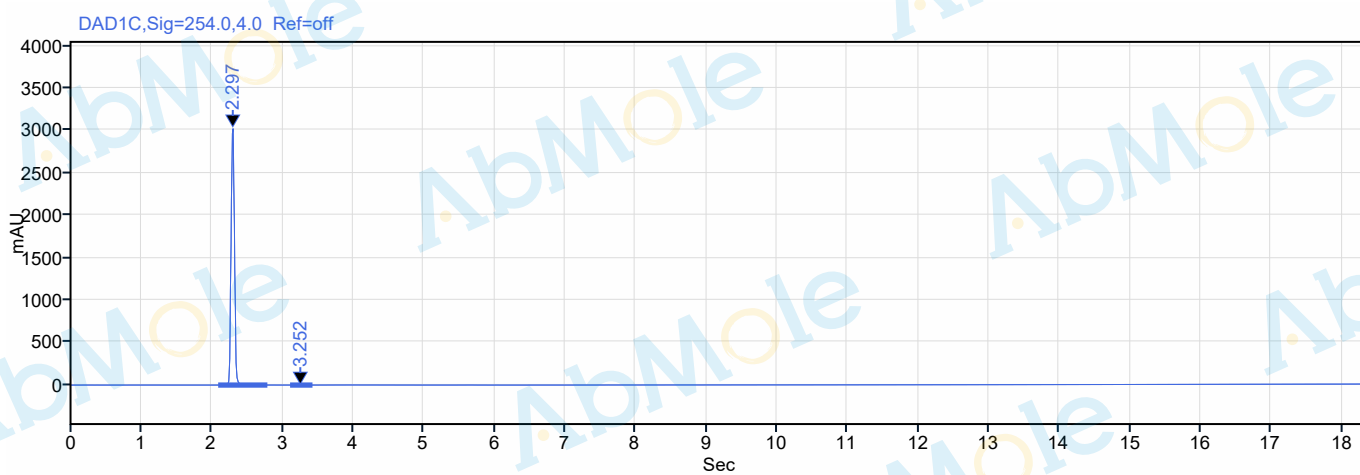

Signal: DAD1C,Sig=254.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
2.297		0.70	10173.8	3036.1	99.90
3.252		0.32	9.7	1.2	0.10