




Sample name: M2312-AG-1478-01
Instrument: A010
Inj. volume: 3
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

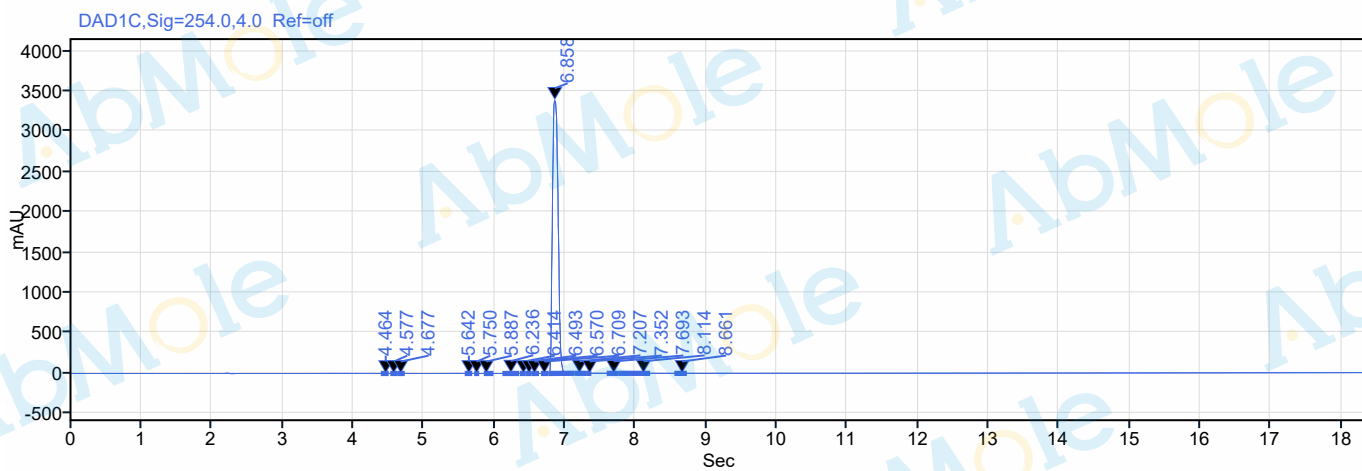

Signal: DAD1C,Sig=254.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
4.464		0.11	0.4	0.1	0.00
4.577		0.10	0.2	0.1	0.00
4.677		0.11	2.2	0.8	0.01
5.642		0.11	2.6	1.0	0.01
5.750		0.07	0.2	0.1	0.00
5.887		0.14	0.5	0.1	0.00
6.236		0.24	21.7	5.7	0.12
6.414		0.08	0.2	0.1	0.00
6.493		0.08	0.3	0.1	0.00
6.570		0.11	0.7	0.2	0.00
6.709		0.11	0.6	0.2	0.00
6.858		0.37	18682.0	3391.2	99.67
7.207		0.16	9.6	2.4	0.05
7.352		0.07	0.3	0.1	0.00
7.693		0.17	2.4	0.6	0.01
8.114		0.44	17.7	2.5	0.09
8.661		0.18	1.9	0.4	0.01