


=====
Acq. Operator : admin
Sample Operator : M2320-17-AAG-06
Acq. Instrument : 3

Location : P2-B-07
Inj : 1
Inj Volume : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl

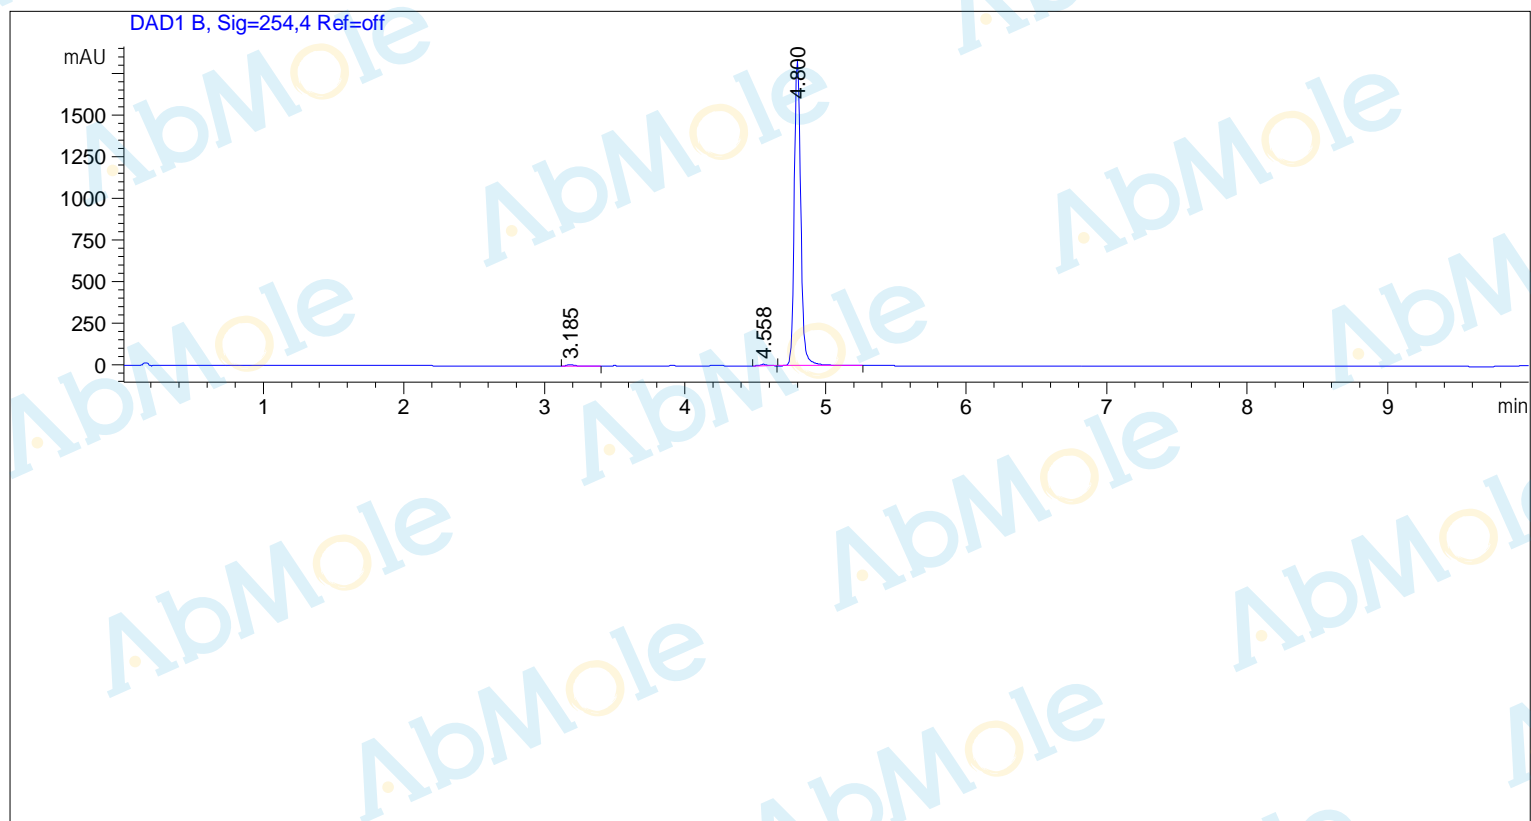

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.185	BB	0.0460	24.56574	8.43609	0.4152
2	4.558	BB	0.0476	25.64425	8.39760	0.4335
3	4.800	BB	0.0515	5865.93604	1826.82715	99.1513

Totals : 5916.14603 1843.66084