



Agilent Technologies

Sample name: M2574-ML161-01

Instrument: A012

Inj. volume: 1.5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

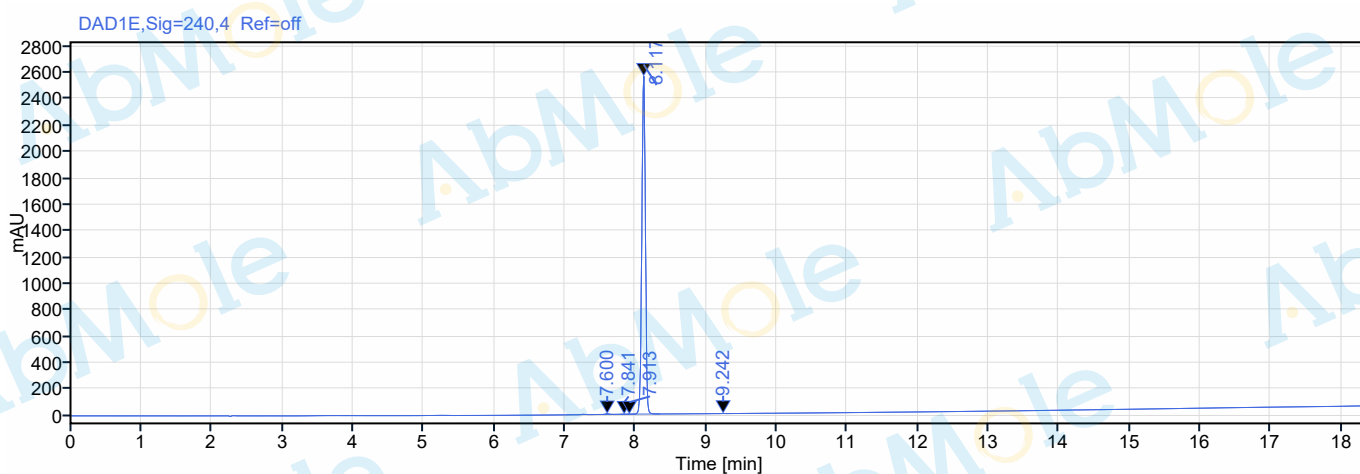

Signal: DAD1E,Sig=240,4 Ref=off

RT [min]	Type	Width [min]	Area	Height	Area%
7.600	MB m	0.14	15.81	5.08	0.17
7.841	MM m	0.07	0.42	0.15	0.00
7.913	MM m	0.07	0.99	0.41	0.01
8.117	BB	0.40	9033.78	2562.31	99.77
9.242	MM m	0.16	3.22	0.78	0.04