



Agilent Technologies

Sample name: M2645-Disopyramide Phosphate-02

Injection date:

Instrument: A012

Location:

Inj. volume: 4


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

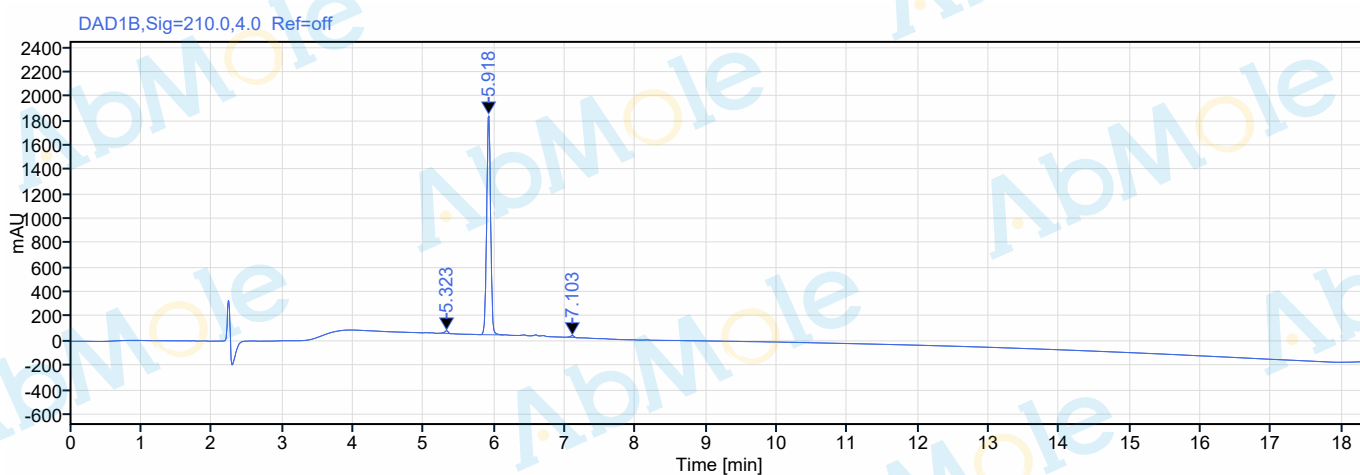

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
5.323	71.41	22.18	1.00
5.918	6997.84	1798.64	98.31
7.103	48.54	15.24	0.68