



Agilent Technologies

Sample name: M2698-Ferrostatin-1-07-1

Instrument: A012

Inj. volume: 10

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

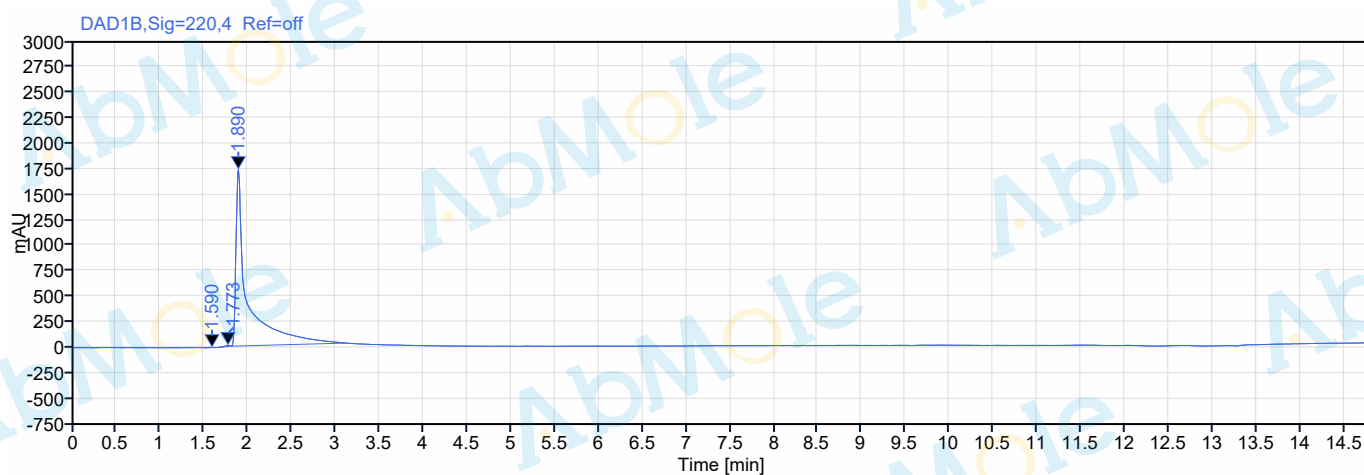

Signal: DAD1B,Sig=220,4 Ref=off

RT [min]	Area	Height	Area%
1.590	4.26	1.16	0.03
1.773	42.72	11.58	0.27
1.890	15907.92	1731.96	99.71