

8.632  
8.304  
8.297  
8.282  
8.275  
7.866  
7.696  
7.674  
7.651  
7.454  
7.435  
7.415  
7.285  
7.266  
7.248  
7.229

1.586

0.024




Current Data Parameters  
NAME GW9662-03  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20210325  
Time\_ 12.40  
INSTRUM spect  
PROBHD 5 mm PADUL 13C  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 8  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 199.46  
DW 62.400 usec  
DE 6.50 usec  
TE 297.3 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 400.1324710 MHz  
NUC1 1H  
P1 10.00 usec  
PLW1 20.00000000 W

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

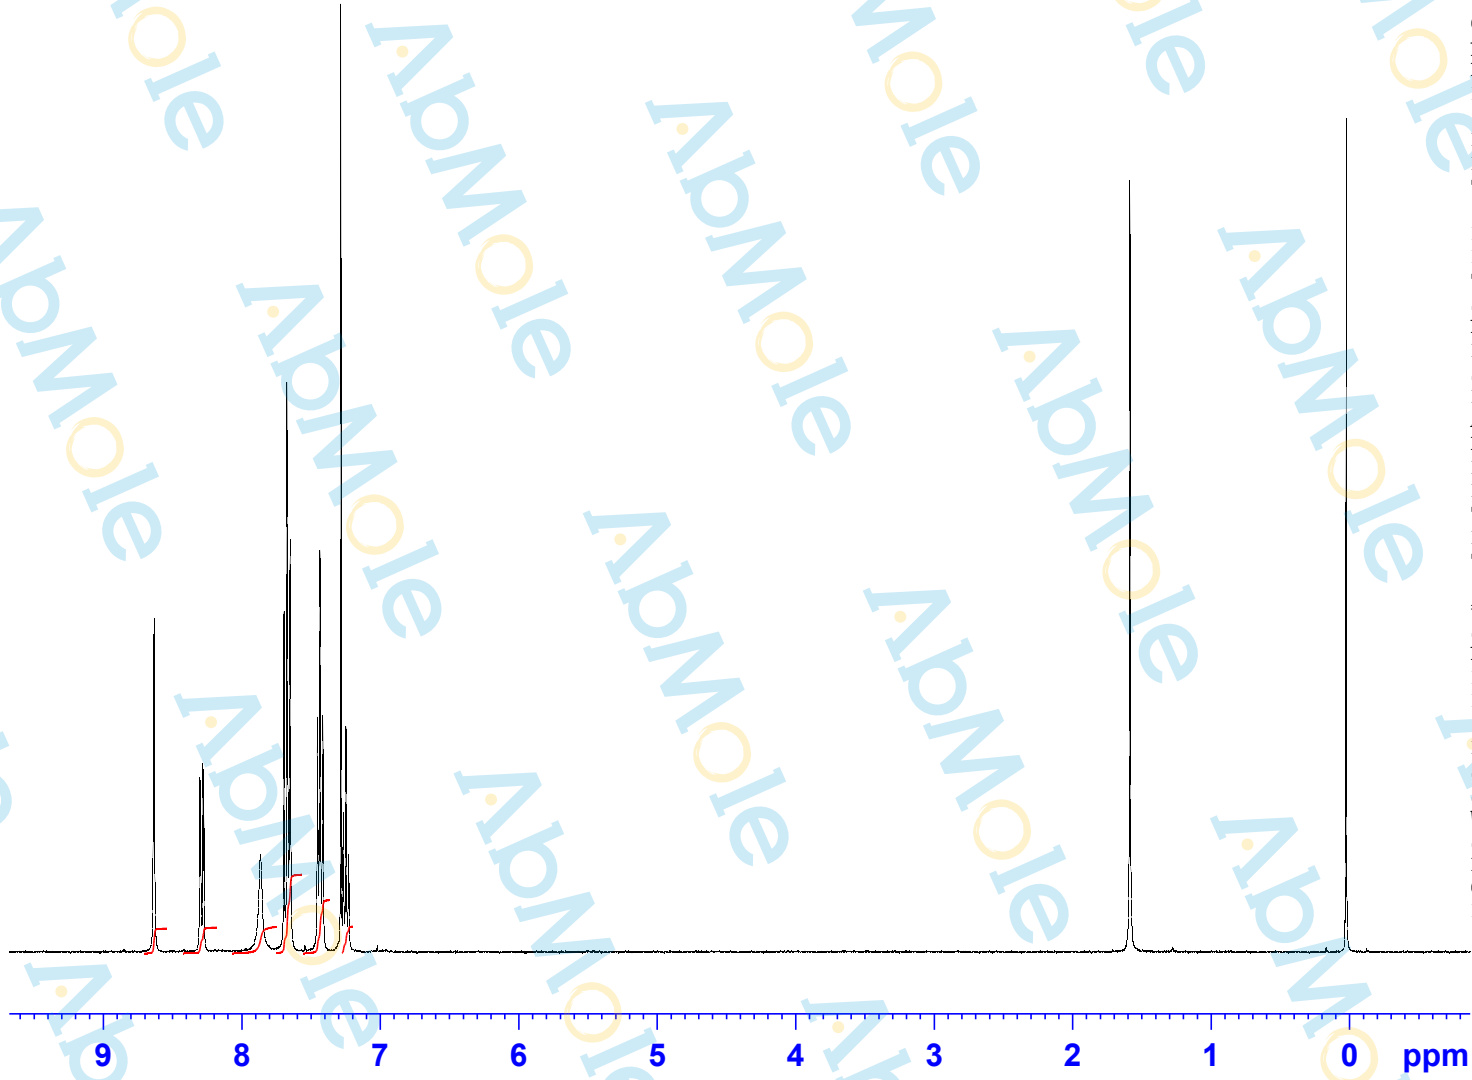

1.00  
1.05  
1.08  
3.17  
2.15  
1.09

9 8 7 6 5 4 3 2 1 0 ppm