



Agilent Technologies

Sample name: M27828-ALW-II-49-7-01

Instrument: A010

Inj. volume: 1.5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

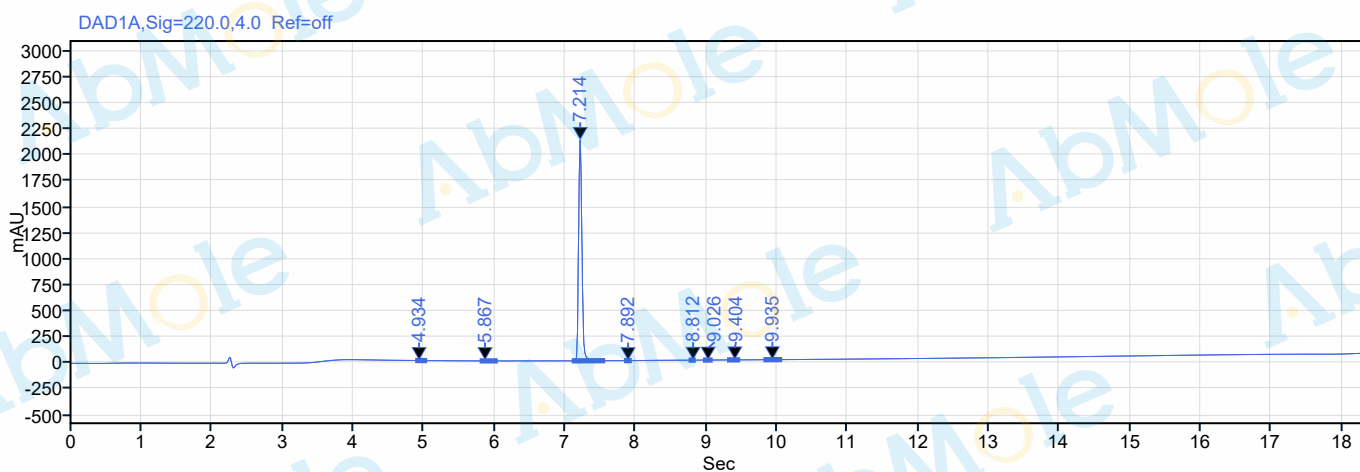

Signal: DAD1A,Sig=220.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
4.934		7.1	2.2	0.100
5.867		15.4	5.0	0.218
7.214		7016.9	2121.4	99.392
7.892		3.5	1.2	0.049
8.812		0.8	0.3	0.012
9.026		2.6	0.7	0.036
9.404		6.7	1.6	0.095
9.935		6.9	1.1	0.098