


```

=====
Acq. Operator   : admin
Sample Operator : M2818-L-NAME hydrochloride-13
Acq. Instrument : 3
Location       : P2-C-07
Inj            : 1
Inj Volume    : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 6.000 µl
=====

```

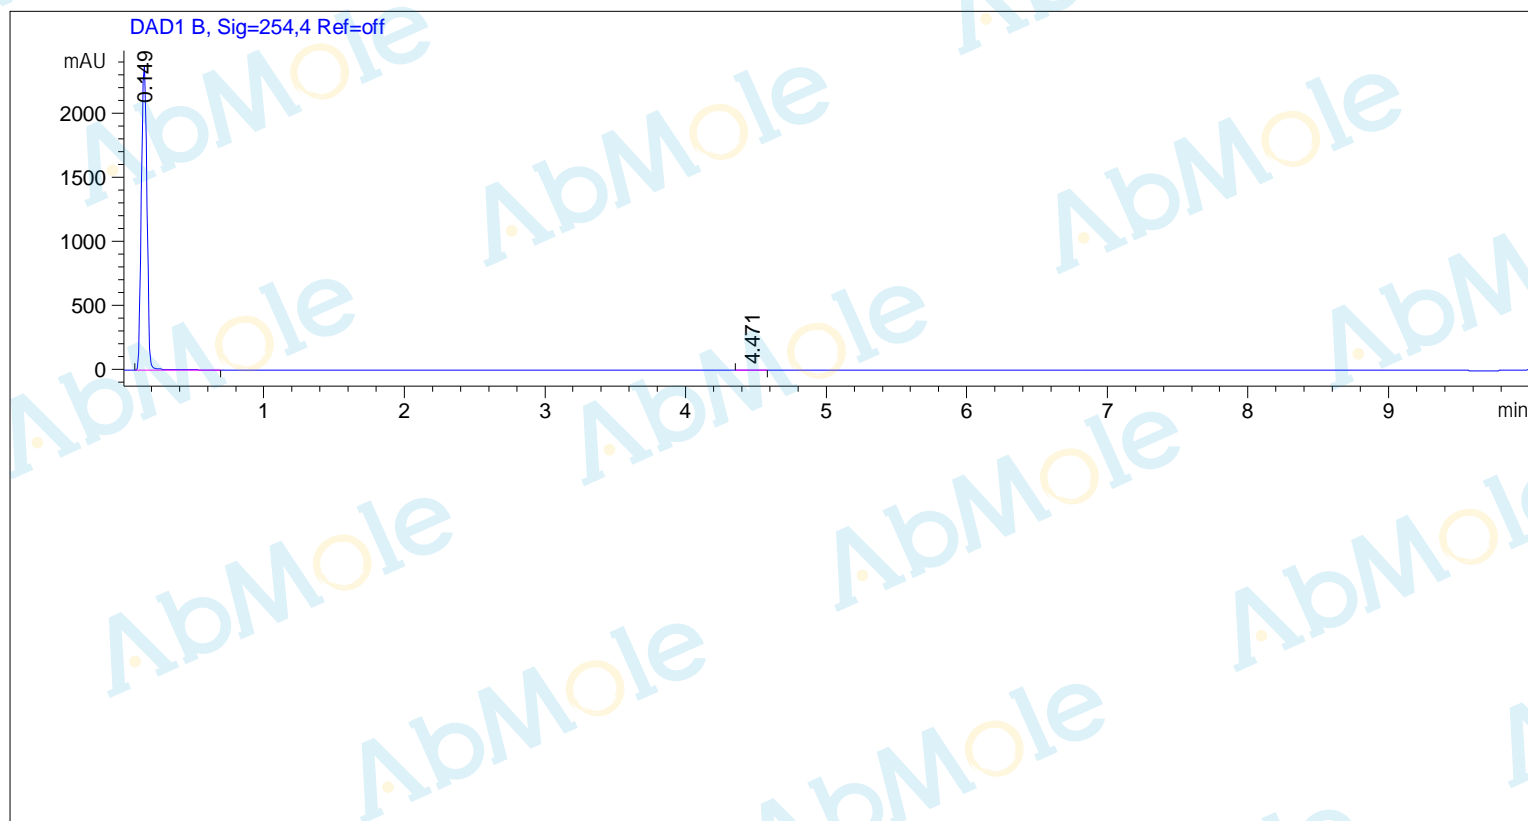

```

=====
                          Area Percent Report
=====

```

```

Sorted By      : Signal
Multiplier    : 1.0000
Dilution      : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.149	BB	0.0439	6484.80713	2375.35791	99.9354
2	4.471	MM	0.1447	4.19335	4.83032e-1	0.0646

```
Totals :                6489.00048 2375.84094
```