




Agilent Technologies

Sample name: M2981-Rimonabant-01
Instrument: A012
Inj. volume: 1
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

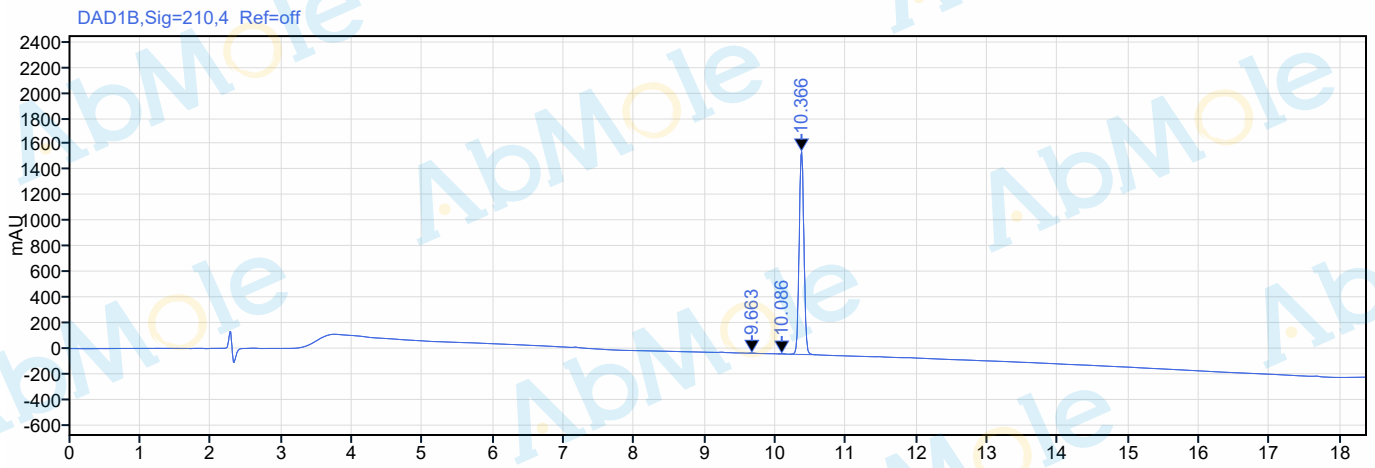

Signal: DAD1B,Sig=210,4 Ref=off

RT [min]	Area	Height	Area%
9.663	6.60	1.83	0.09
10.086	5.22	1.49	0.07
10.366	7491.54	1588.72	99.84