


=====
Acq. Operator : admin
Sample Operator : M3010-Sirtinol-01
Acq. Instrument : 3

Location : P2-D-11
Inj : 1
Inj Volume : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl

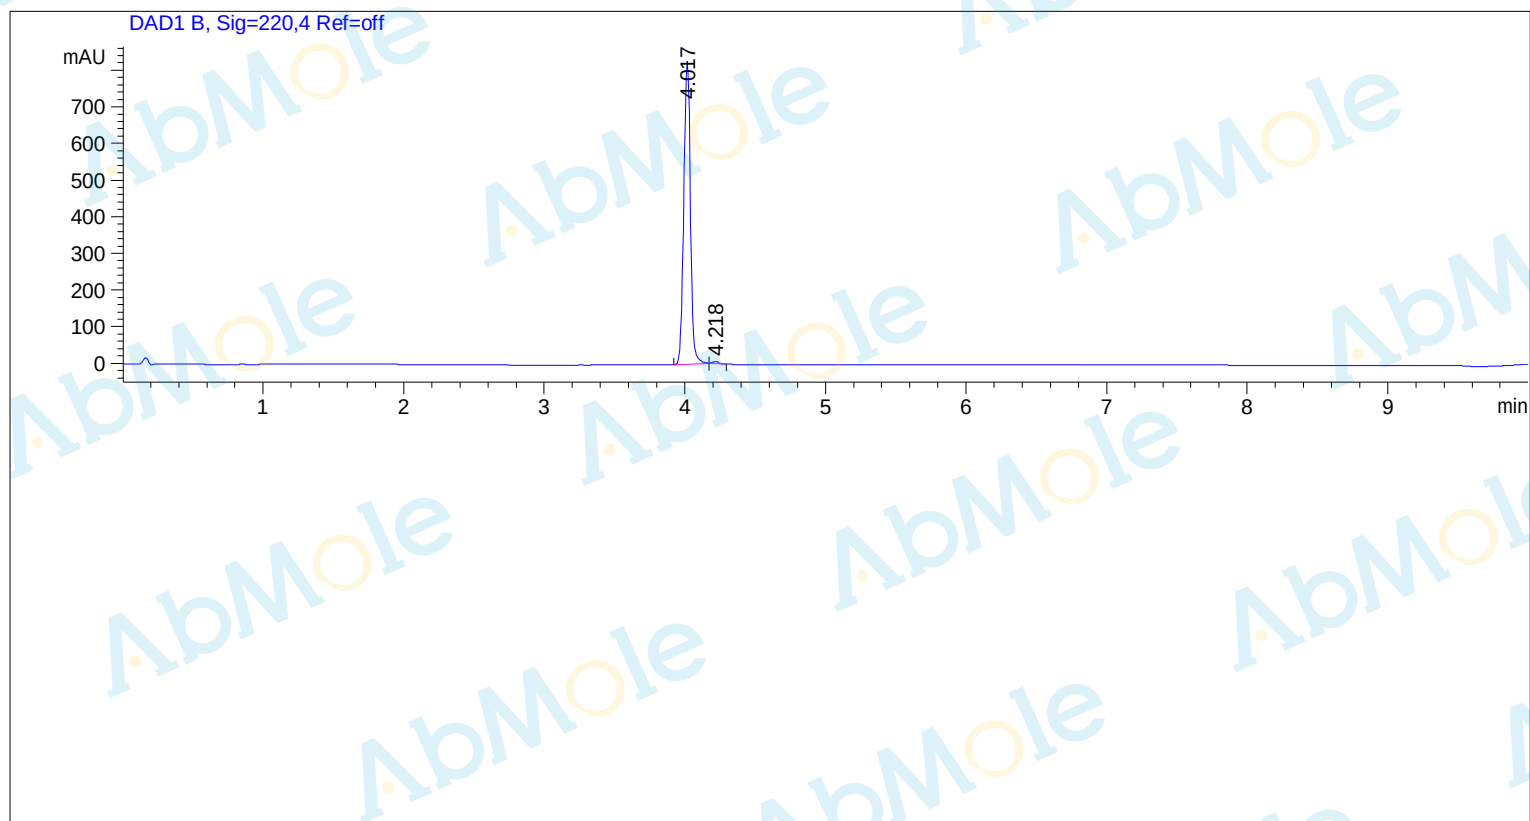

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.017	BB	0.0523	2713.73999	826.60272	99.4204
2	4.218	BB	0.0444	15.81947	5.69950	0.5796

Totals : 2729.55946 832.30222